

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
 Data File : P0046213.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2018 16:42
 Operator : SM/UA
 Sample : J3627-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 26KV-CC-6

Manual Integrations
 APPROVED

ugo
 6/26/2018 10:09:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 17:23:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 25 12:49:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.609	6870687	2469255	11.755	9.948
2) SA Decachlor...	10.046	8.576	7205833	2758854	15.629	16.493m
Target Compounds						
31) L7 AR-1260-1	7.140	6.163	3486915	1613395	123.417	130.860
32) L7 AR-1260-2	7.395	6.350	6040769	2014216	182.120	135.634 #
33) L7 AR-1260-3	7.676	6.677	9739032	3656357	249.141	232.467
34) L7 AR-1260-4	8.287	7.210	5640586	2622270	106.987	112.702
35) L7 AR-1260-5	8.605	7.555	4022515	1994161	124.506	117.491

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 16:42
Operator : SM/UA
Sample : J3627-11
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
26KV-CC-6


Manual Integrations
APPROVED

ugo
6/26/2018 10:09:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 17:23:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:49:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

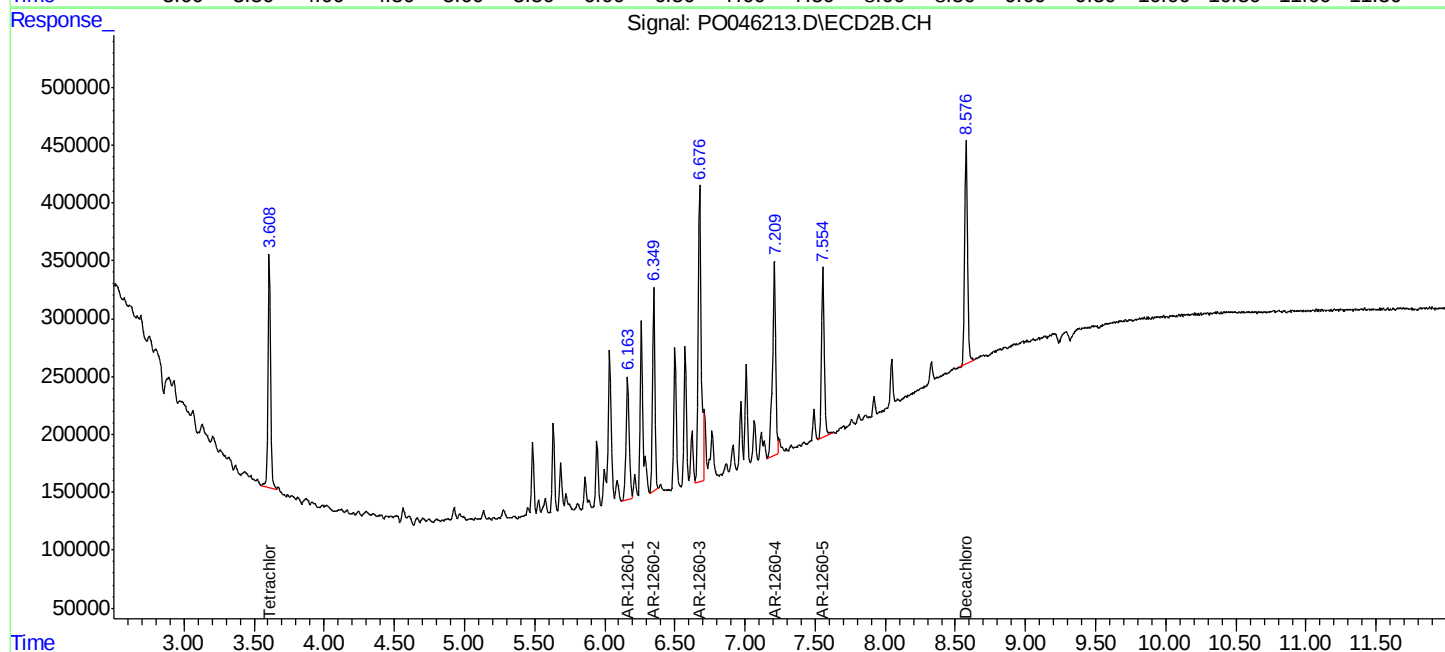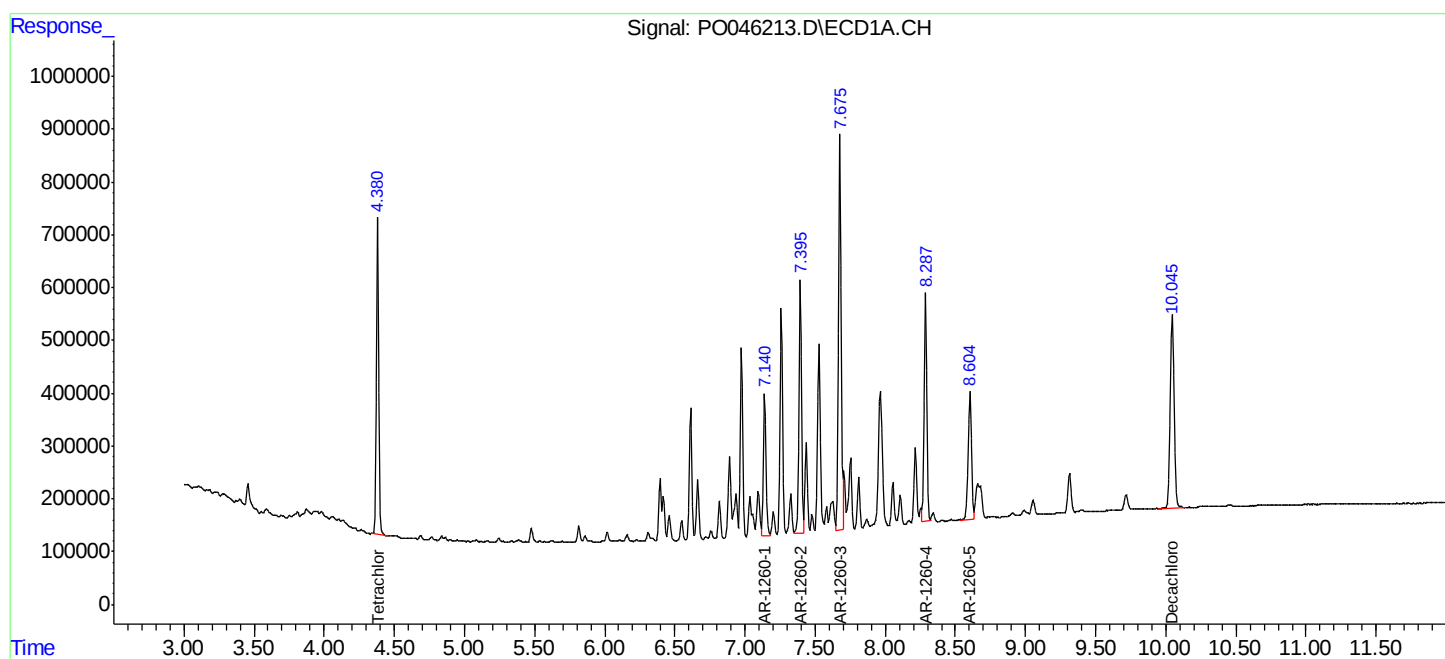

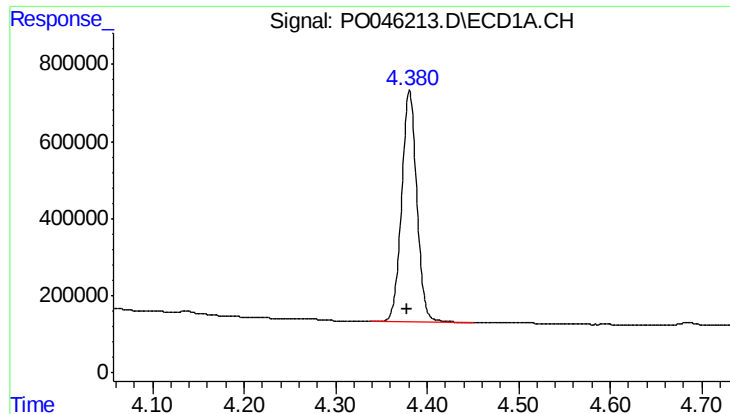


#1 Tetrachloro-m-xylene

R.T.: 4.381 min
Delta R.T.: 0.003 min
Response: 6870687
Conc: 11.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-CC-6


Manual Integrations
APPROVED

ugo
6/26/2018 10:09:47 AM

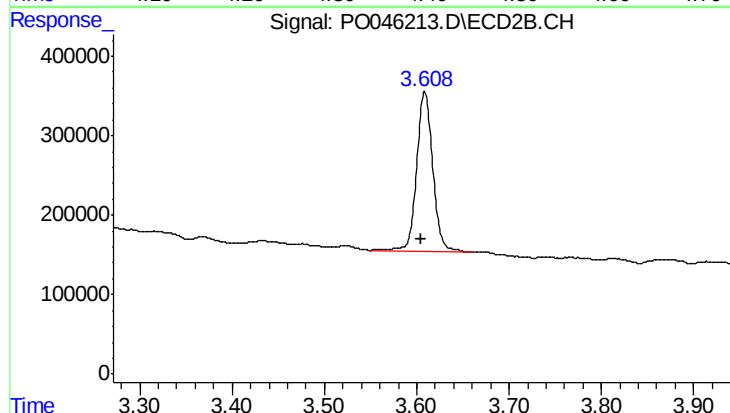


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: 0.004 min
Response: 2469255
Conc: 9.95 ng/ml

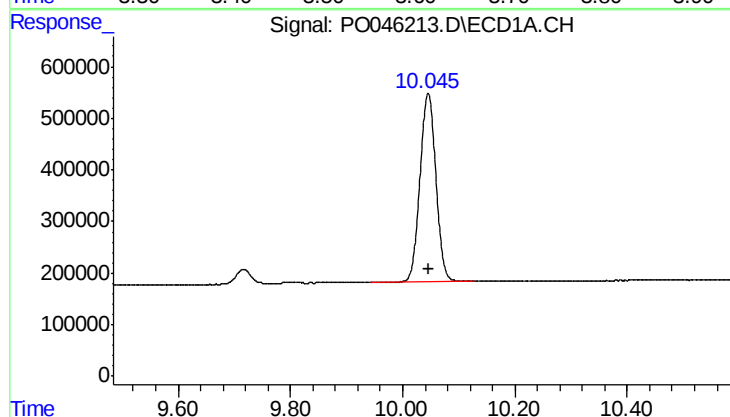


#2 Decachlorobiphenyl

R.T.: 10.046 min
Delta R.T.: -0.001 min
Response: 7205833
Conc: 15.63 ng/ml

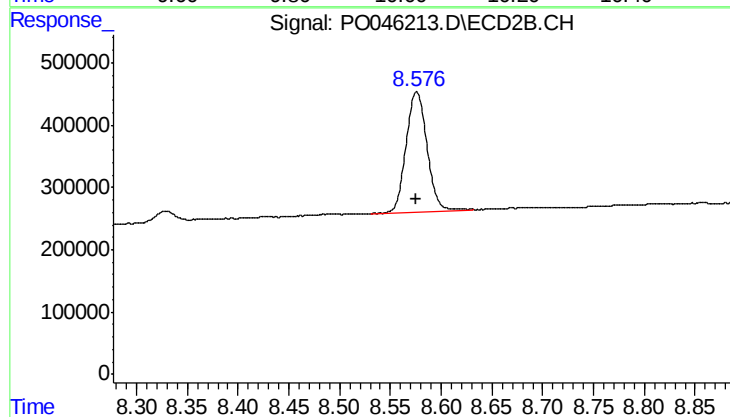

#2 Decachlorobiphenyl

R.T.: 8.576 min
Delta R.T.: 0.000 min
Response: 2758854
Conc: 16.49 ng/ml m

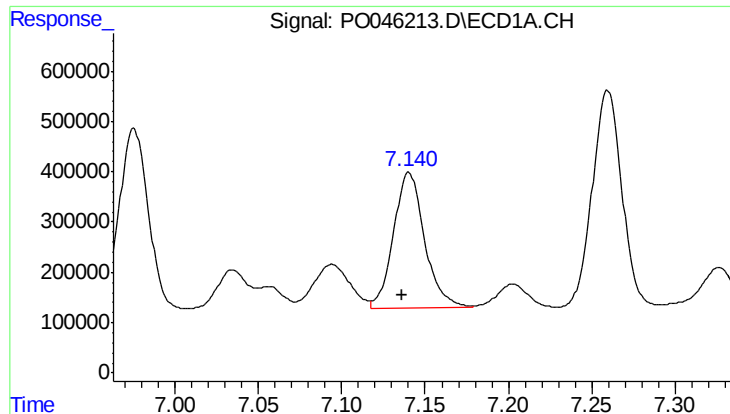


#31 AR-1260-1

R.T.: 7.140 min
Delta R.T.: 0.004 min
Response: 3486915
Conc: 123.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-CC-6


Manual Integrations
APPROVED

ugo
6/26/2018 10:09:47 AM

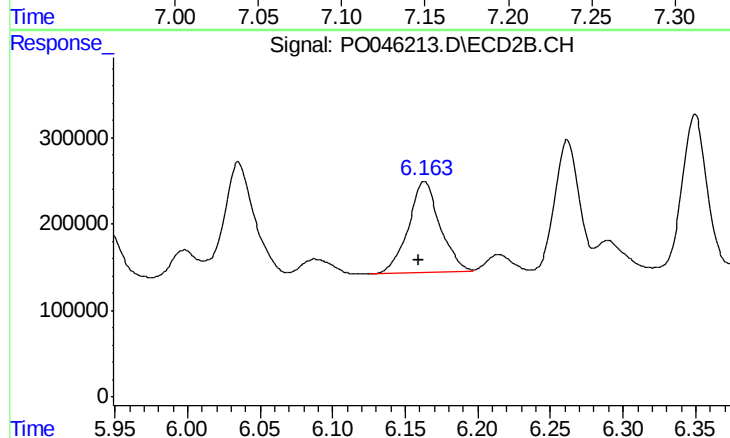


#31 AR-1260-1

R.T.: 6.163 min
Delta R.T.: 0.004 min
Response: 1613395
Conc: 130.86 ng/ml

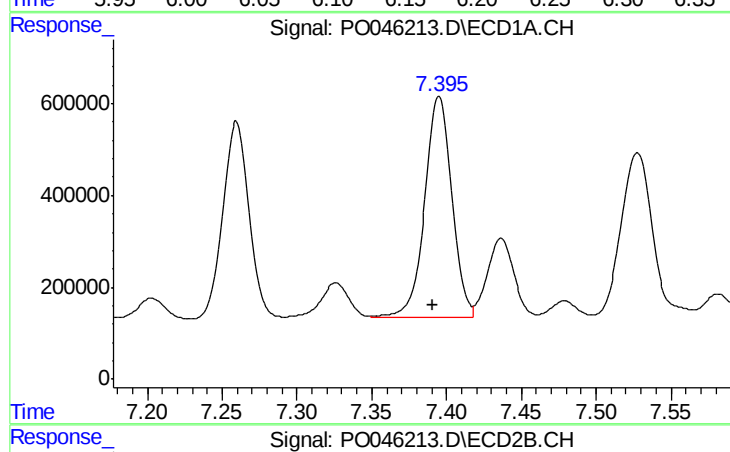


#32 AR-1260-2

R.T.: 7.395 min
Delta R.T.: 0.004 min
Response: 6040769
Conc: 182.12 ng/ml

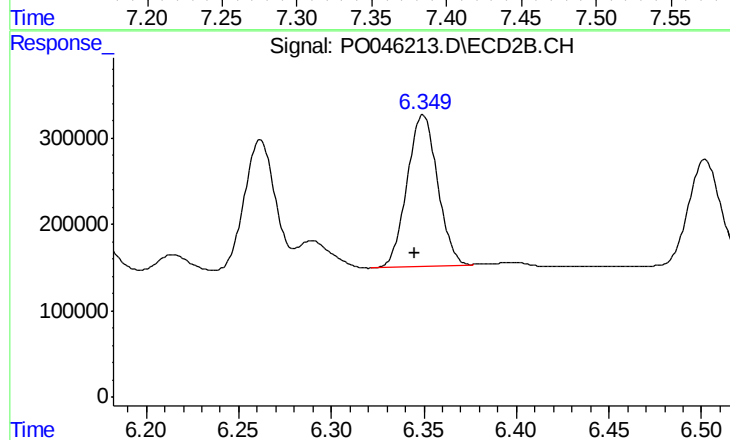

#32 AR-1260-2

R.T.: 6.350 min
Delta R.T.: 0.004 min
Response: 2014216
Conc: 135.63 ng/ml

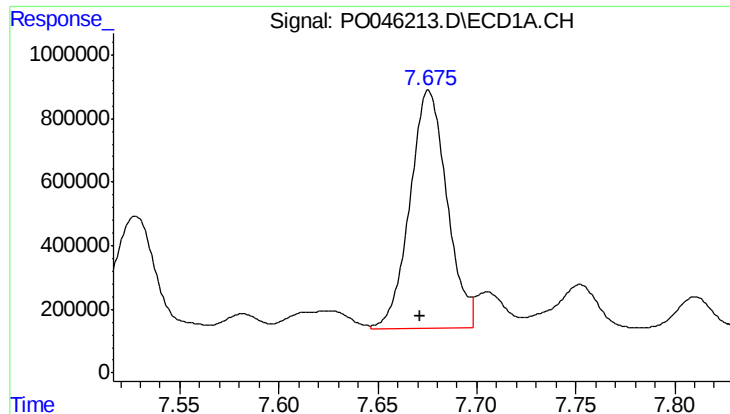


#33 AR-1260-3

R.T.: 7.676 min
Delta R.T.: 0.005 min
Response: 9739032
Conc: 249.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-CC-6


Manual Integrations
APPROVED

ugo
6/26/2018 10:09:47 AM

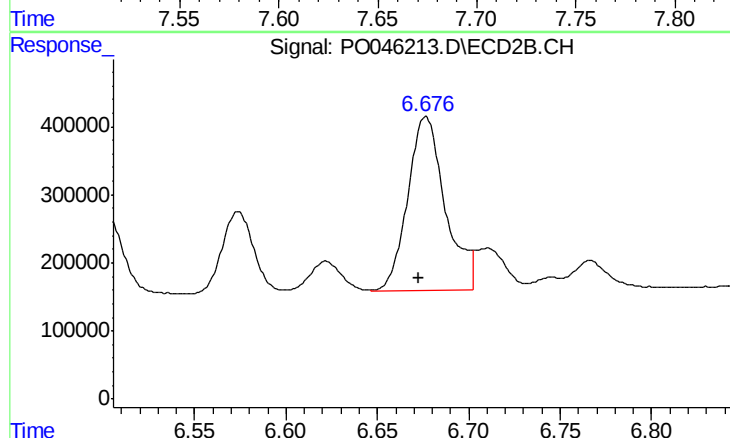


#33 AR-1260-3

R.T.: 6.677 min
Delta R.T.: 0.004 min
Response: 3656357
Conc: 232.47 ng/ml

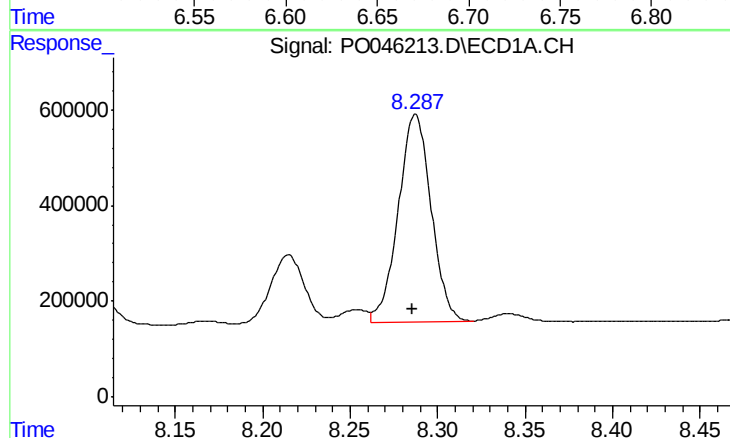


#34 AR-1260-4

R.T.: 8.287 min
Delta R.T.: 0.002 min
Response: 5640586
Conc: 106.99 ng/ml

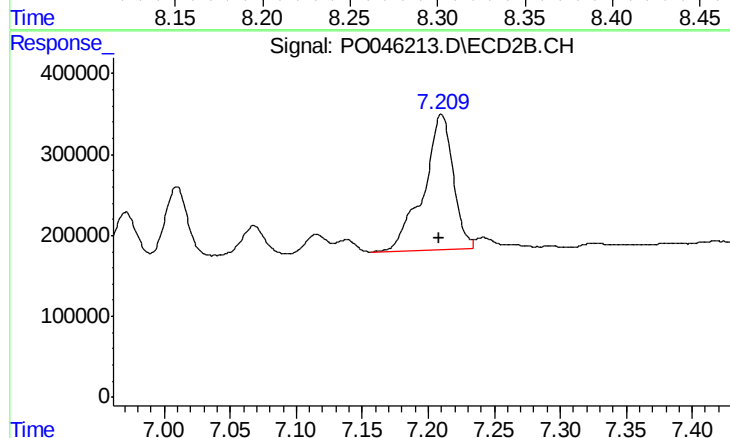

#34 AR-1260-4

R.T.: 7.210 min
Delta R.T.: 0.002 min
Response: 2622270
Conc: 112.70 ng/ml

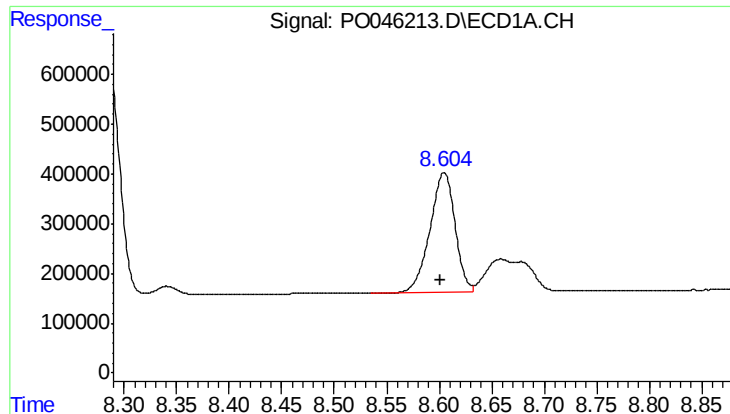


#35 AR-1260-5

R.T.: 8.605 min
Delta R.T.: 0.003 min
Response: 4022515
Conc: 124.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-CC-6

Manual Integrations
APPROVED

ugo
6/26/2018 10:09:47 AM

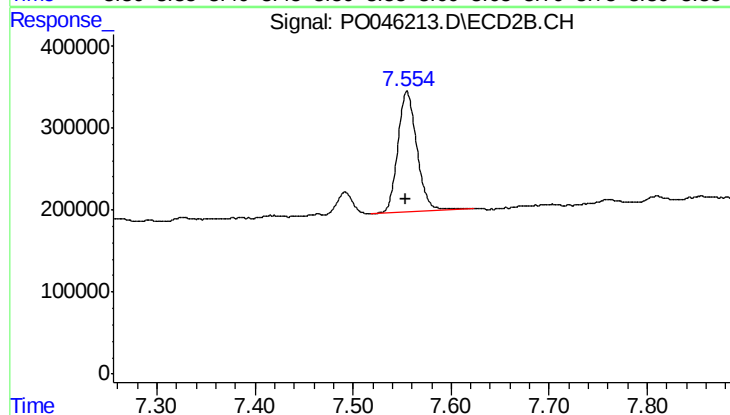

#35 AR-1260-5

R.T.: 7.555 min
Delta R.T.: 0.002 min
Response: 1994161
Conc: 117.49 ng/ml