

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
 Data File : P0046217.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2018 18:03
 Operator : SM/UA
 Sample : J3627-35 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GROUND-WATER

Manual Integrations
 APPROVED

ugo
 6/26/2018 10:10:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 18:23:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 25 12:49:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.605	1116374	573925	1.910m	2.312
2) SA Decachlor...	10.065	8.580	680344	262130	1.476m	1.567m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046217.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 18:03
Operator : SM/UA
Sample : J3627-35 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 18:23:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:49:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

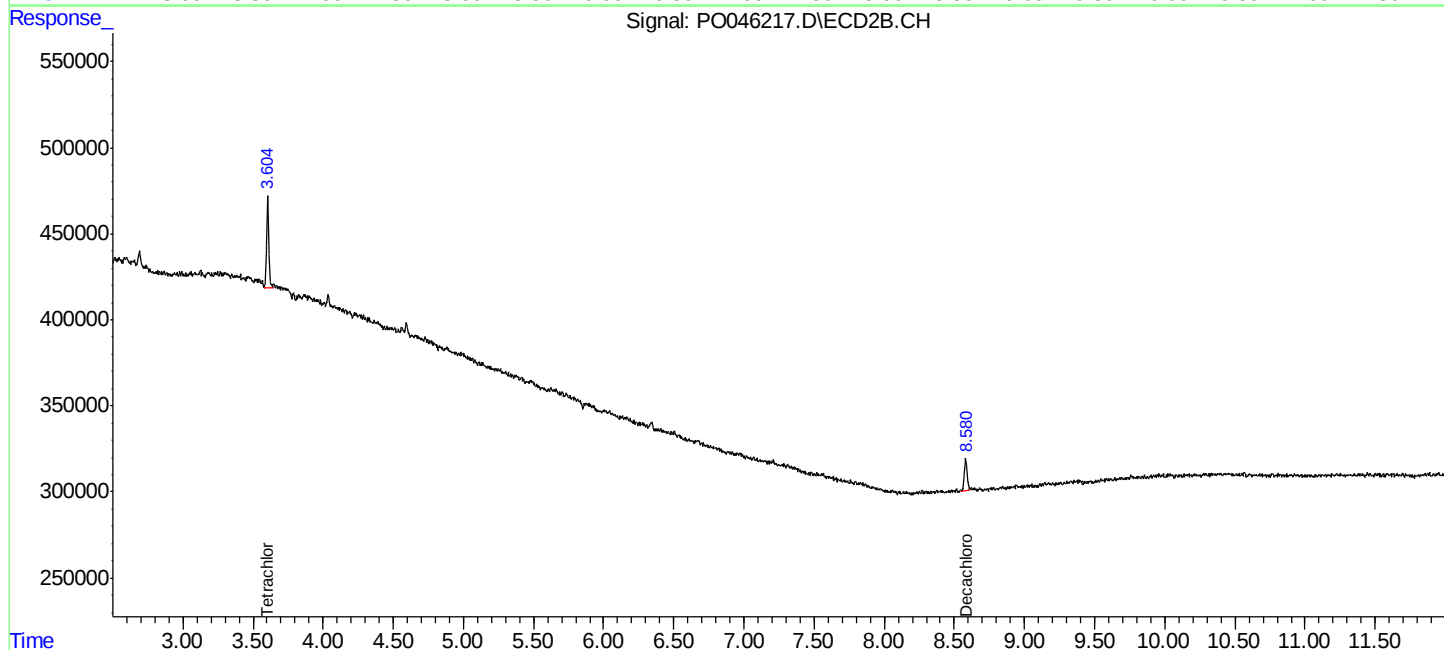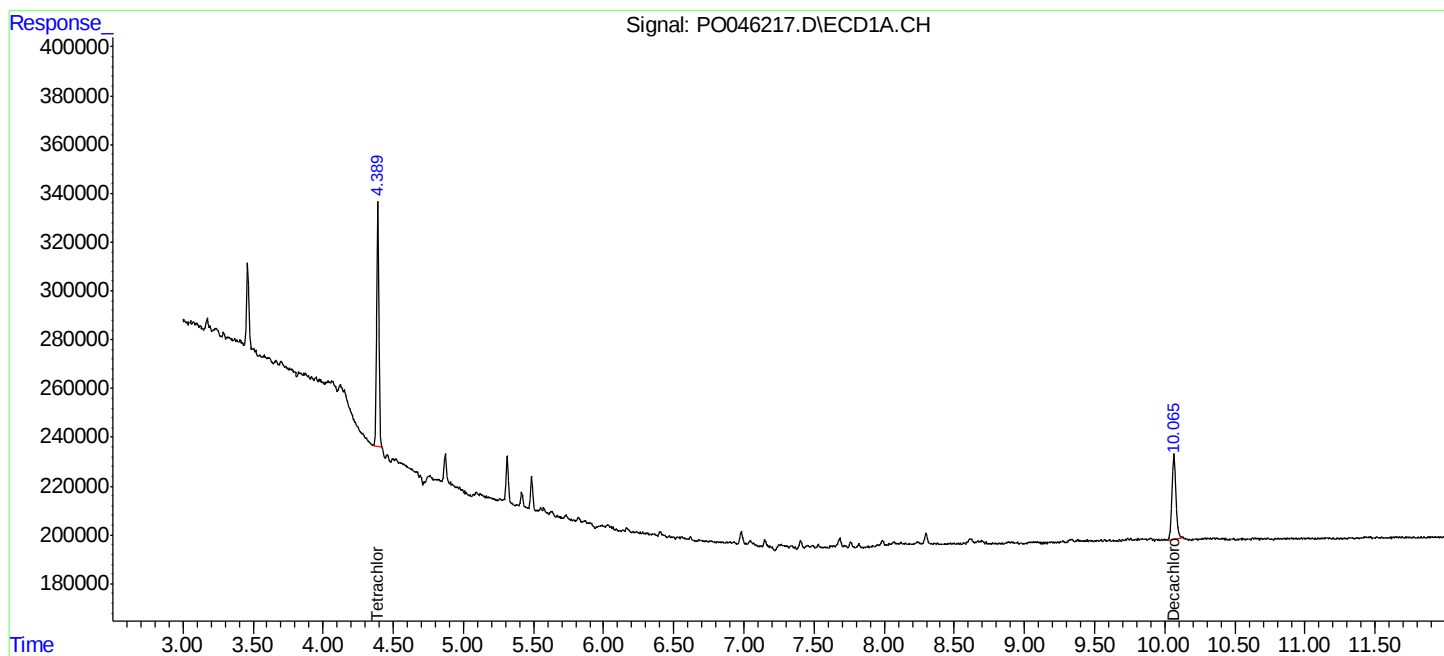

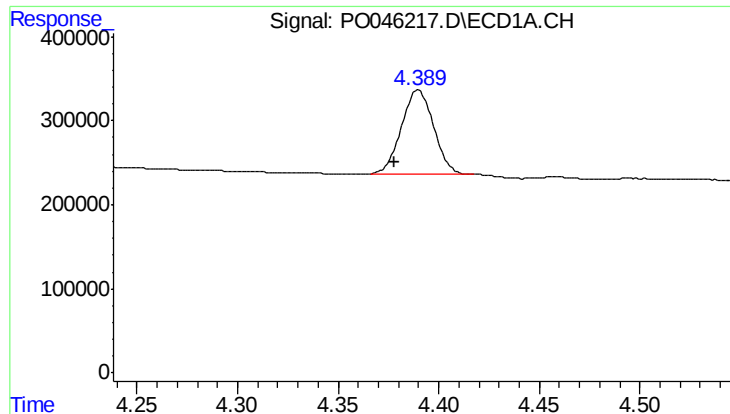


#1 Tetrachloro-m-xylene

R.T.: 4.389 min
Delta R.T.: 0.011 min
Response: 1116374
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:12 AM

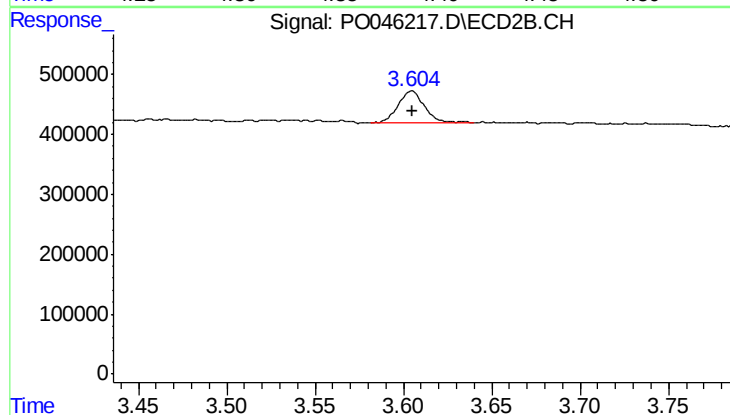


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 573925
Conc: 2.31 ng/ml

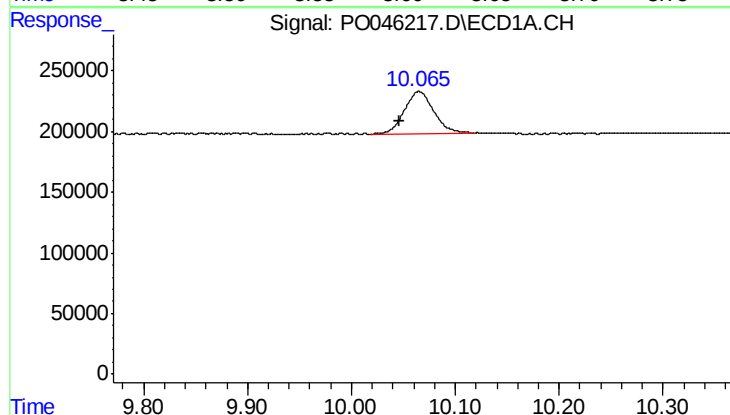

#2 Decachlorobiphenyl

R.T.: 10.065 min
Delta R.T.: 0.018 min
Response: 680344
Conc: 1.48 ng/ml m

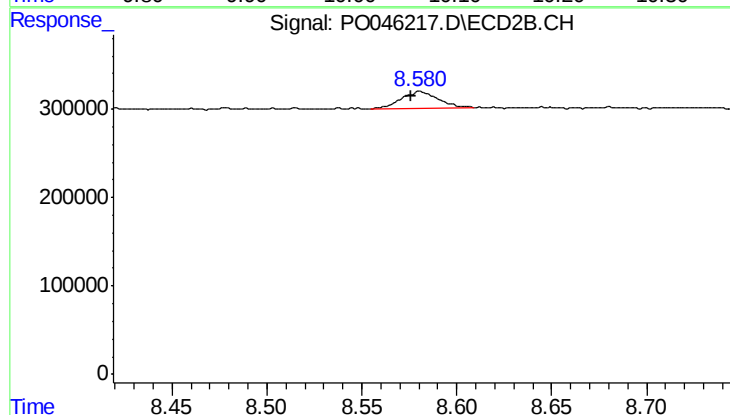

#2 Decachlorobiphenyl

R.T.: 8.580 min
Delta R.T.: 0.004 min
Response: 262130
Conc: 1.57 ng/ml m