

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
 Data File : P0046224.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2018 20:05
 Operator : SM/UA
 Sample : J3570-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20180373-AMENDED-COMPOSITE-

Manual Integrations
 APPROVED

ugo
 6/26/2018 10:10:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:10:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 25 12:44:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.379	3.606	8980421	4027548	15.599	16.406
2) SA Decachlor...	10.047	8.574	6183448	2380940	13.656	14.478m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046224.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 20:05
Operator : SM/UA
Sample : J3570-10
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20180373-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:10:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:44:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

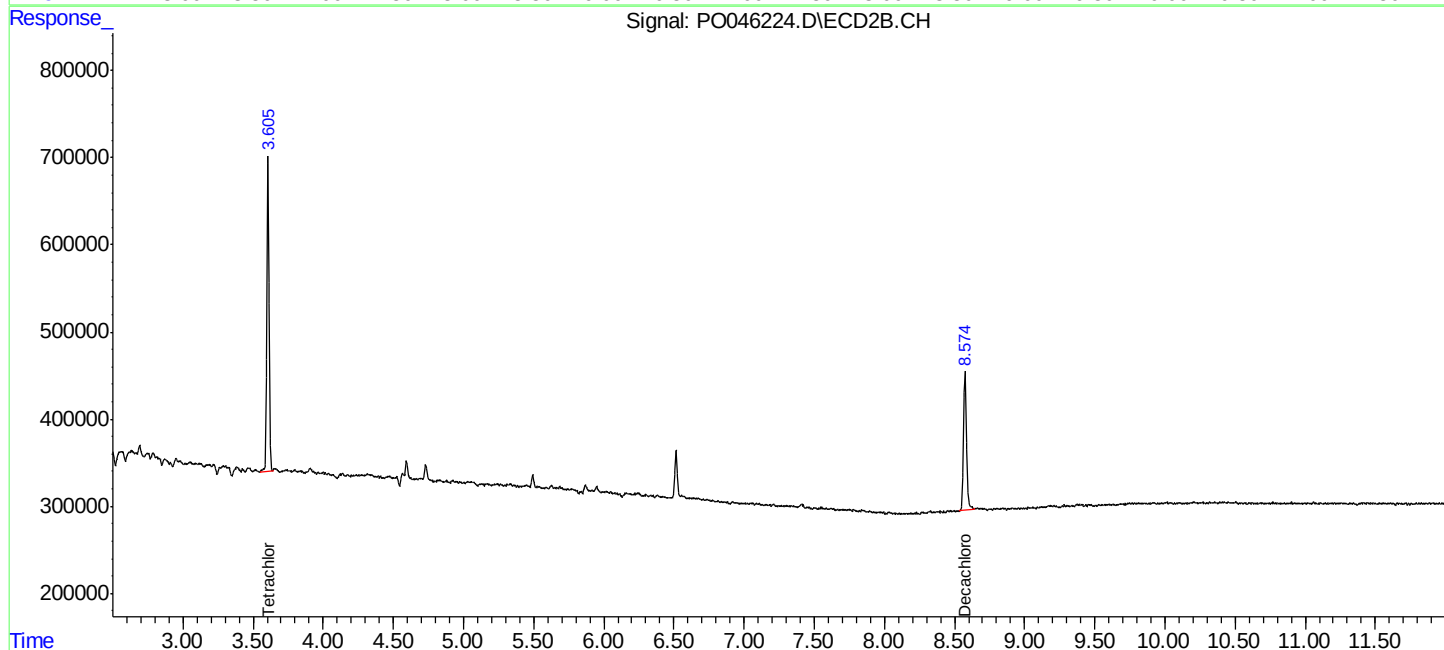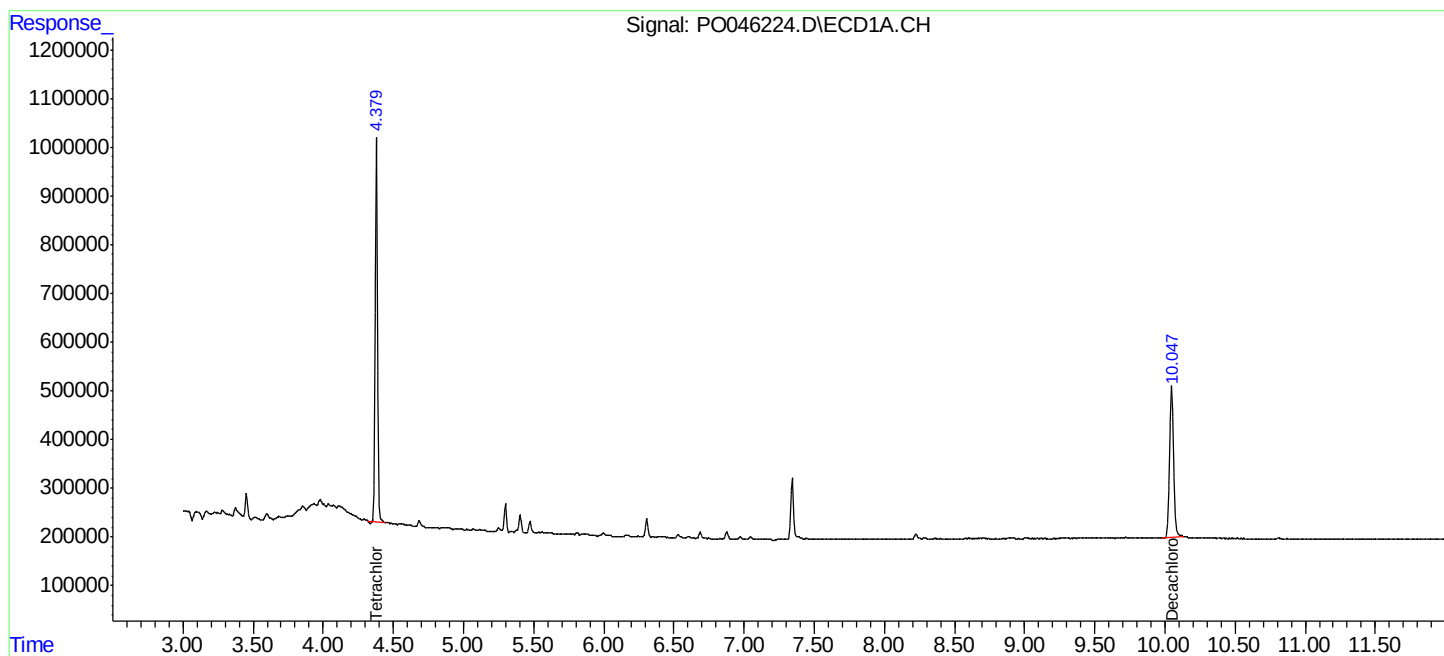

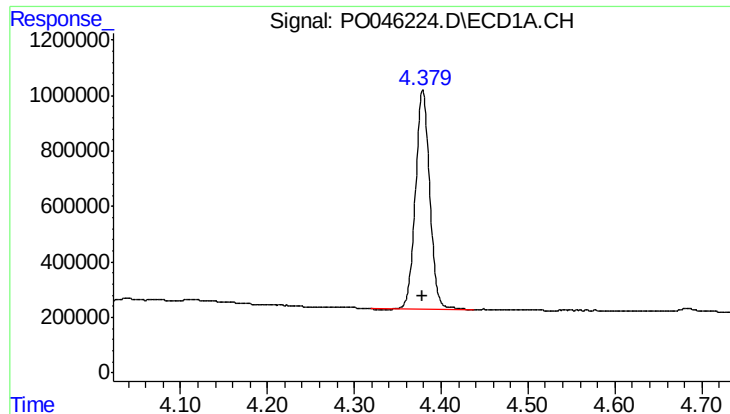


#1 Tetrachloro-m-xylene

R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 8980421
Conc: 15.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
20180373-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:25 AM

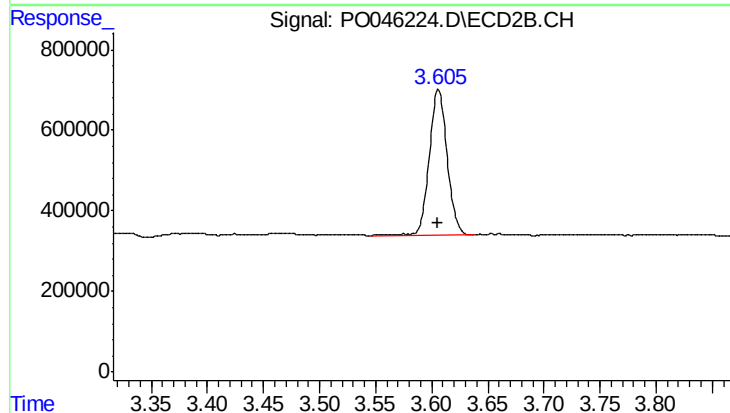


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 4027548
Conc: 16.41 ng/ml

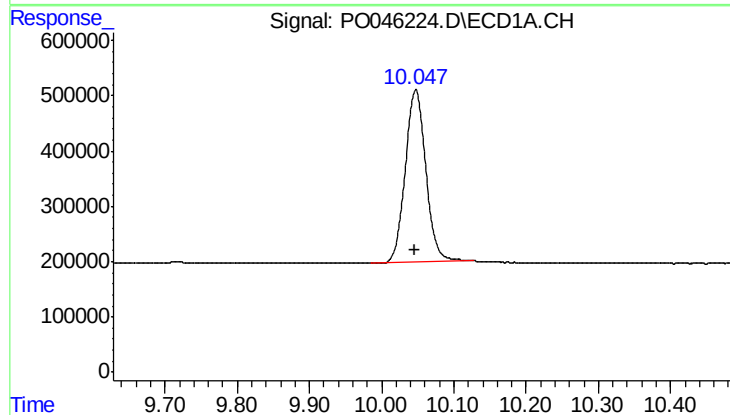

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: 0.001 min
Response: 6183448
Conc: 13.66 ng/ml

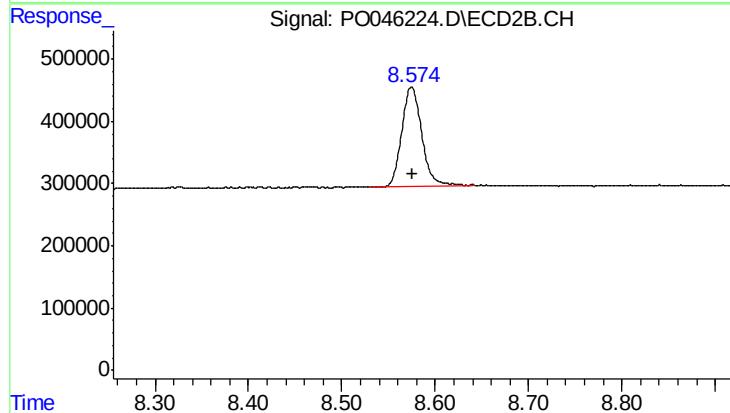

#2 Decachlorobiphenyl

R.T.: 8.574 min
Delta R.T.: -0.002 min
Response: 2380940
Conc: 14.48 ng/ml m