

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 20:21
Operator : SM/UA
Sample : J3570-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20180374-AMENDED-COMPOSITE-

Manual Integrations
APPROVED

ugo
6/26/2018 10:10:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:15:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:44:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.379	3.605	9950707	4109878	17.285m	16.742m
2)	SA Decachlor...	10.047	8.575	6375362	2446836	14.079	14.879

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 20:21
Operator : SM/UA
Sample : J3570-11
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20180374-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:15:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:44:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

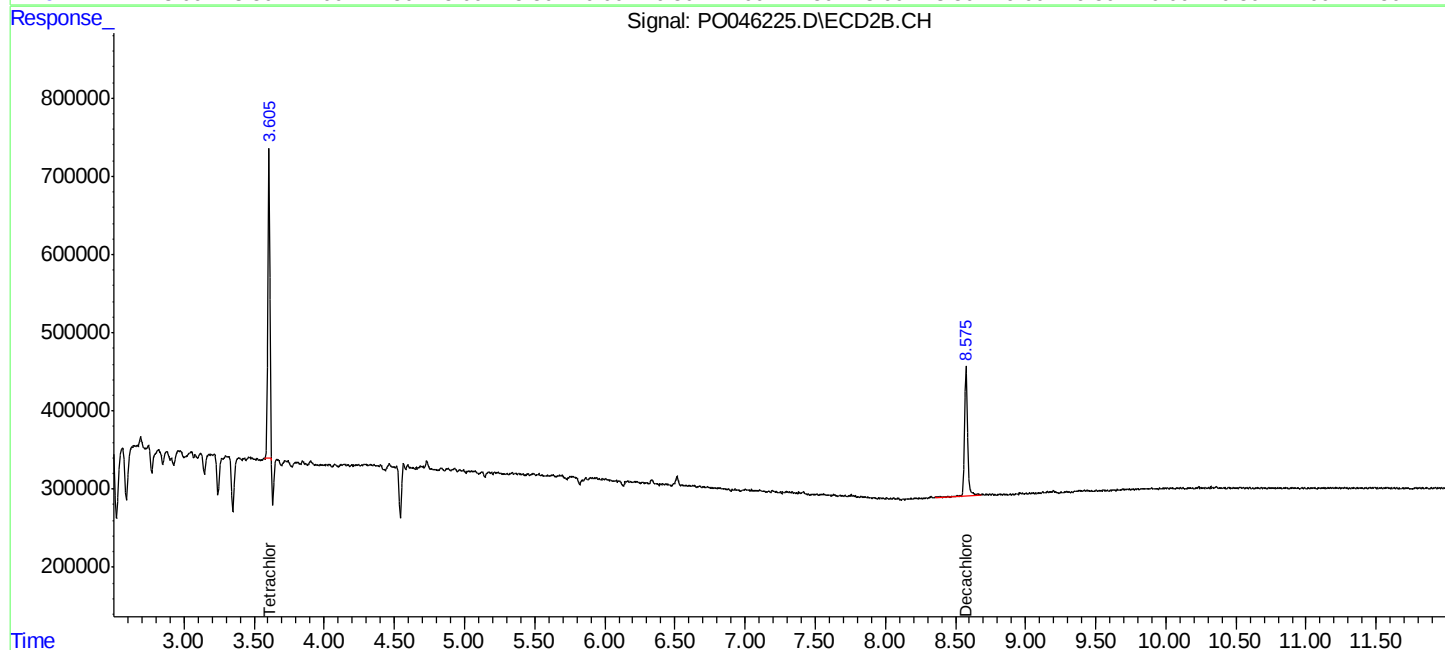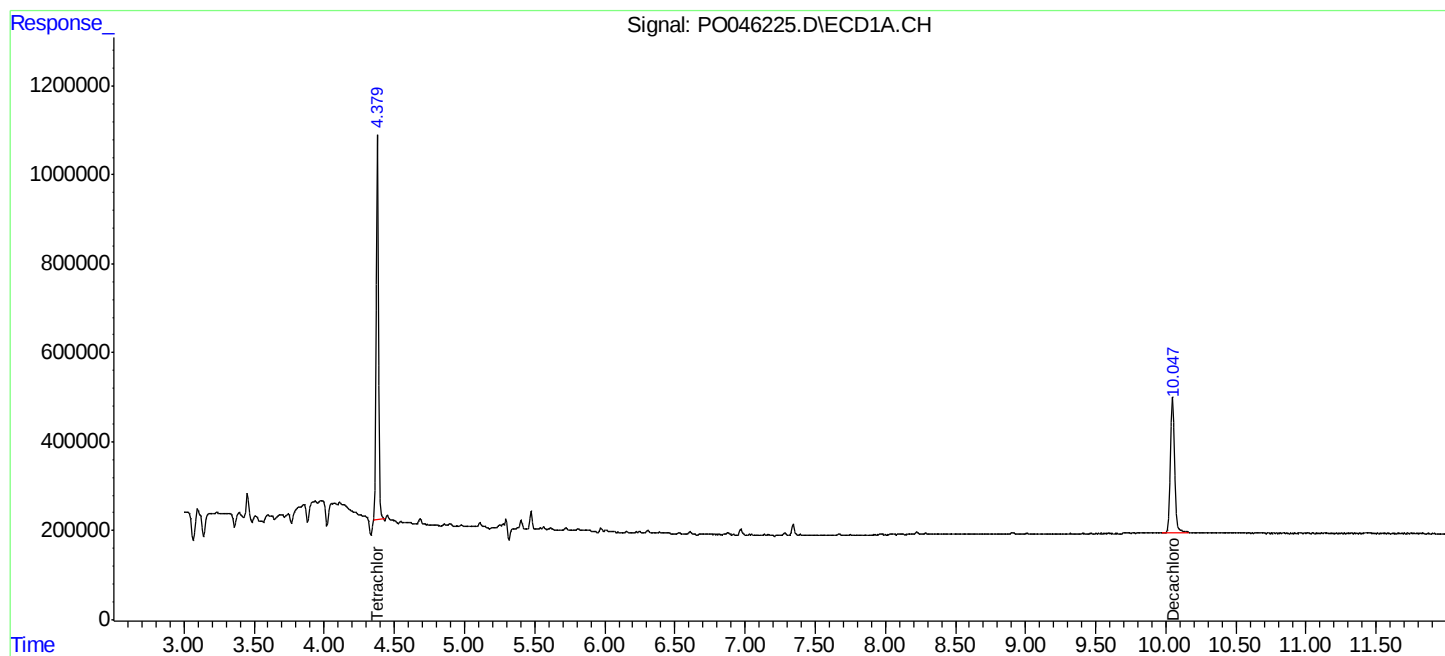

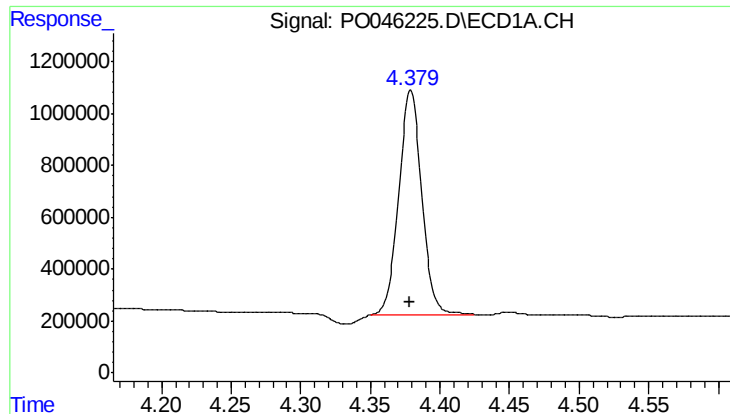


#1 Tetrachloro-m-xylene

R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 9950707
Conc: 17.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
20180374-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:28 AM

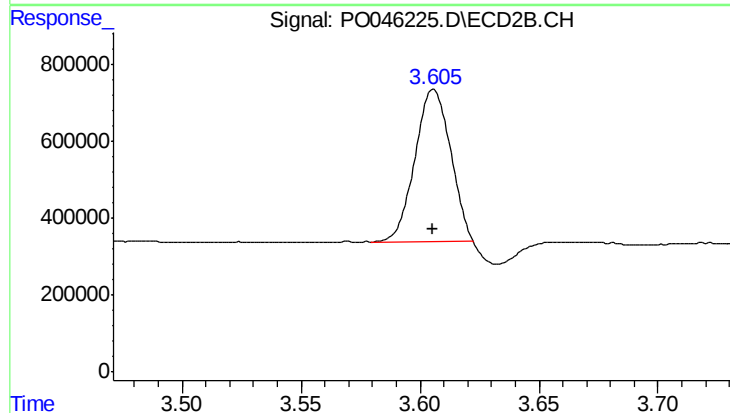


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 4109878
Conc: 16.74 ng/ml m

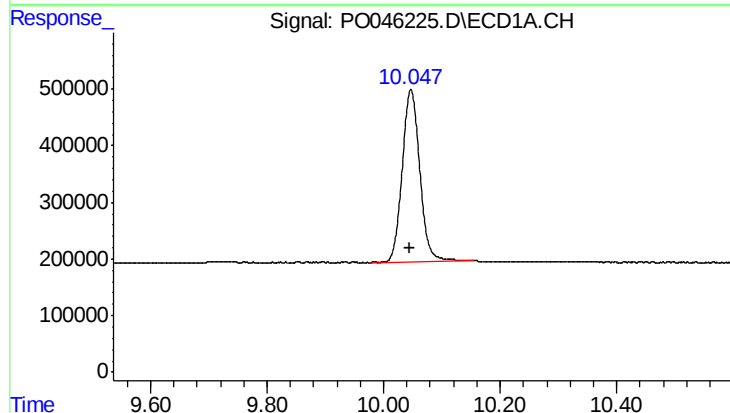

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: 0.001 min
Response: 6375362
Conc: 14.08 ng/ml

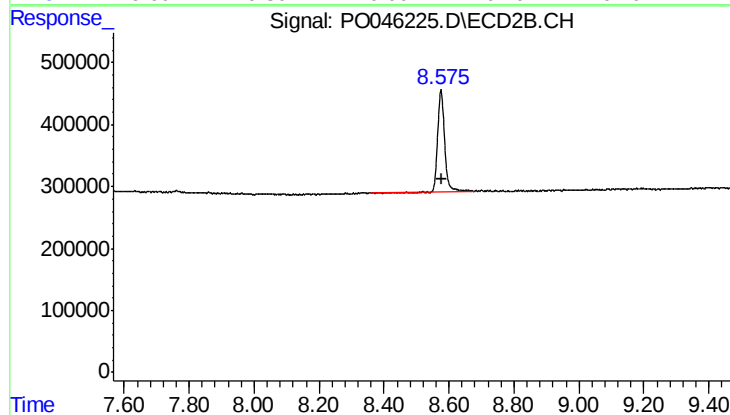

#2 Decachlorobiphenyl

R.T.: 8.575 min
Delta R.T.: 0.000 min
Response: 2446836
Conc: 14.88 ng/ml