

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
 Data File : P0046231.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2018 21:56
 Operator : SM/UA
 Sample : J3241-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-06-062218-B

Manual Integrations
 APPROVED

ugo
 6/26/2018 10:10:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:26:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 25 12:44:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.380	3.608	4981001	2868950	8.652	11.687m#
2) SA Decachlor...	10.045	8.574	3178859	1089043	7.020	6.622m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046231.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 21:56
Operator : SM/UA
Sample : J3241-15
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HR-06-062218-B


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:26:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:44:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

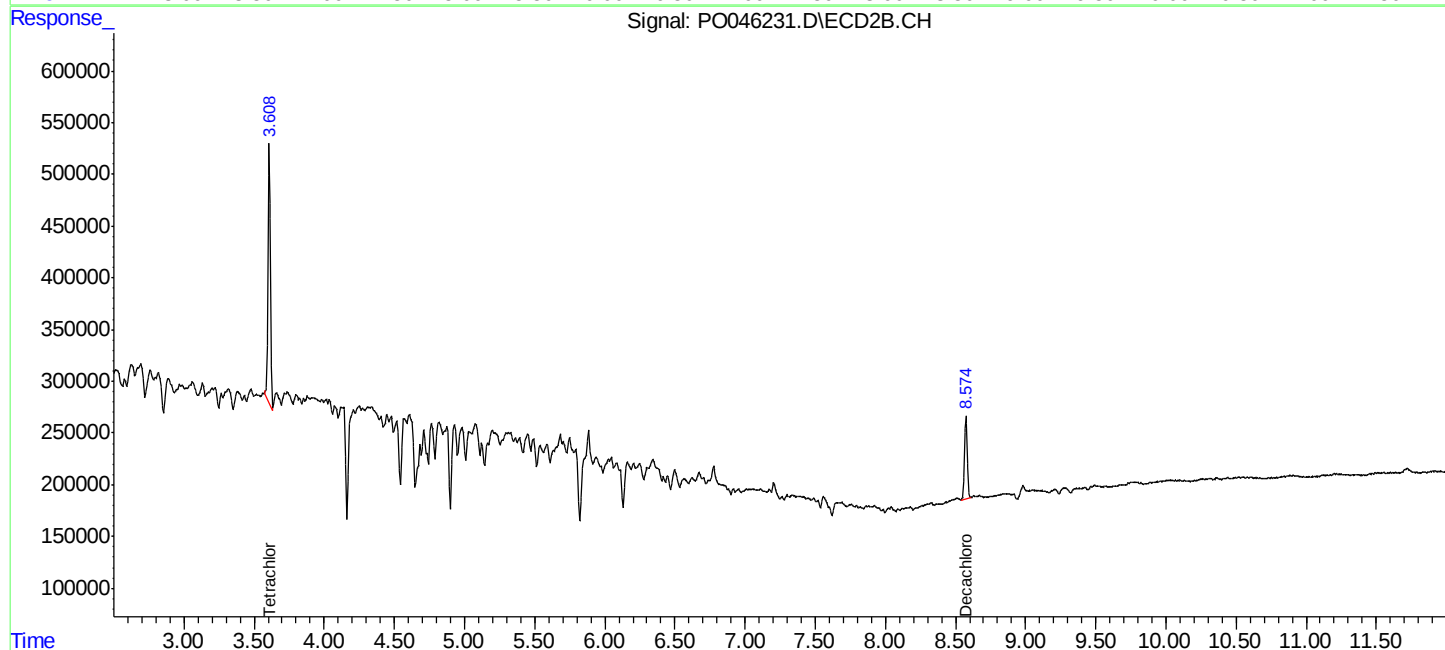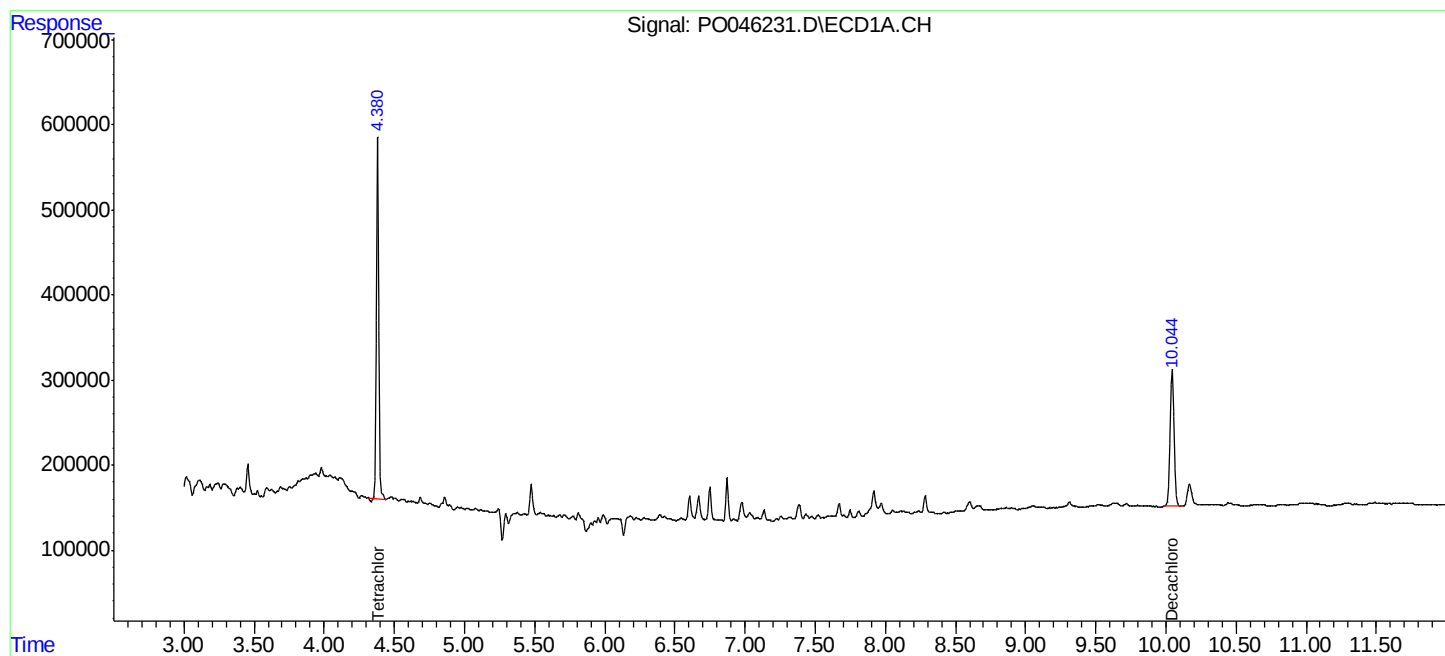

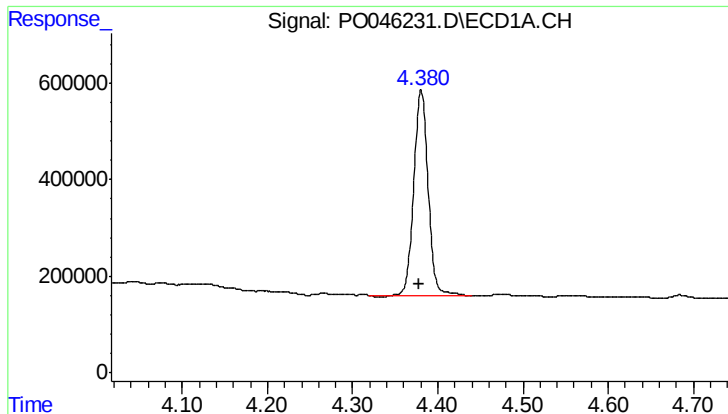


#1 Tetrachloro-m-xylene

R.T.: 4.380 min
Delta R.T.: 0.002 min
Response: 4981001
Conc: 8.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-06-062218-B


Manual Integrations
APPROVED

ugo
6/26/2018 10:10:52 AM

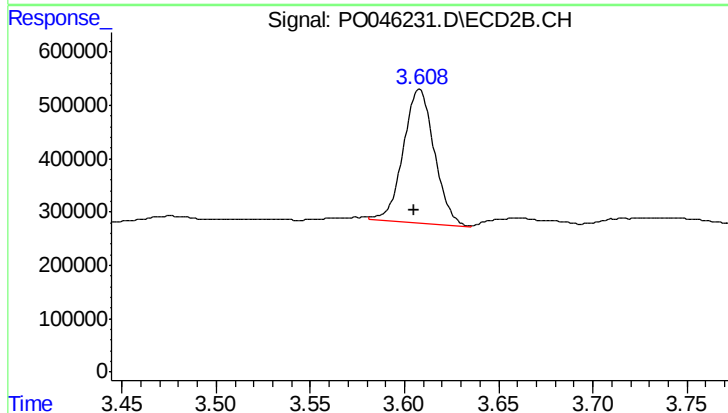


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: 0.002 min
Response: 2868950
Conc: 11.69 ng/ml m

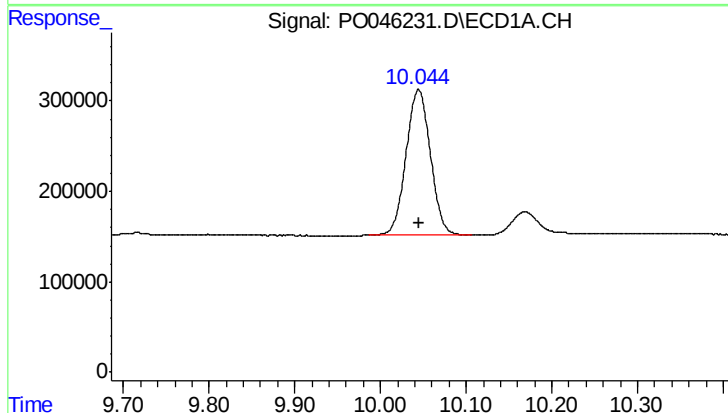

#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.001 min
Response: 3178859
Conc: 7.02 ng/ml

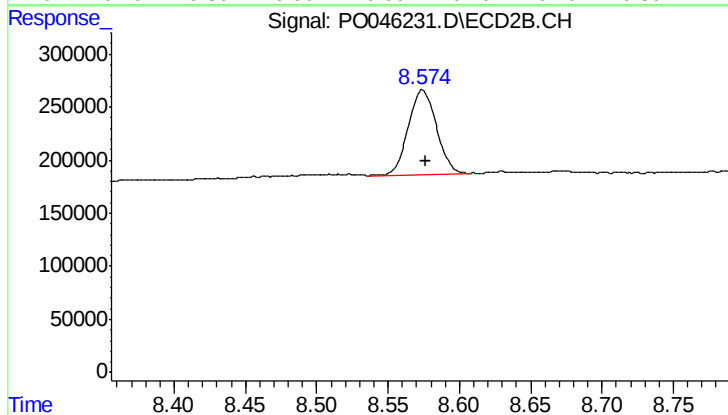

#2 Decachlorobiphenyl

R.T.: 8.574 min
Delta R.T.: -0.003 min
Response: 1089043
Conc: 6.62 ng/ml m