

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046241.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 00:35
Operator : SM/UA
Sample : J3642-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:57:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:44:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.379	3.606	9023823	4049324	15.675	16.495
2) SA Decachlor...	10.044	8.574	5143673	2144429	11.359	13.040

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046241.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 00:35
Operator : SM/UA
Sample : J3642-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:57:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:44:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

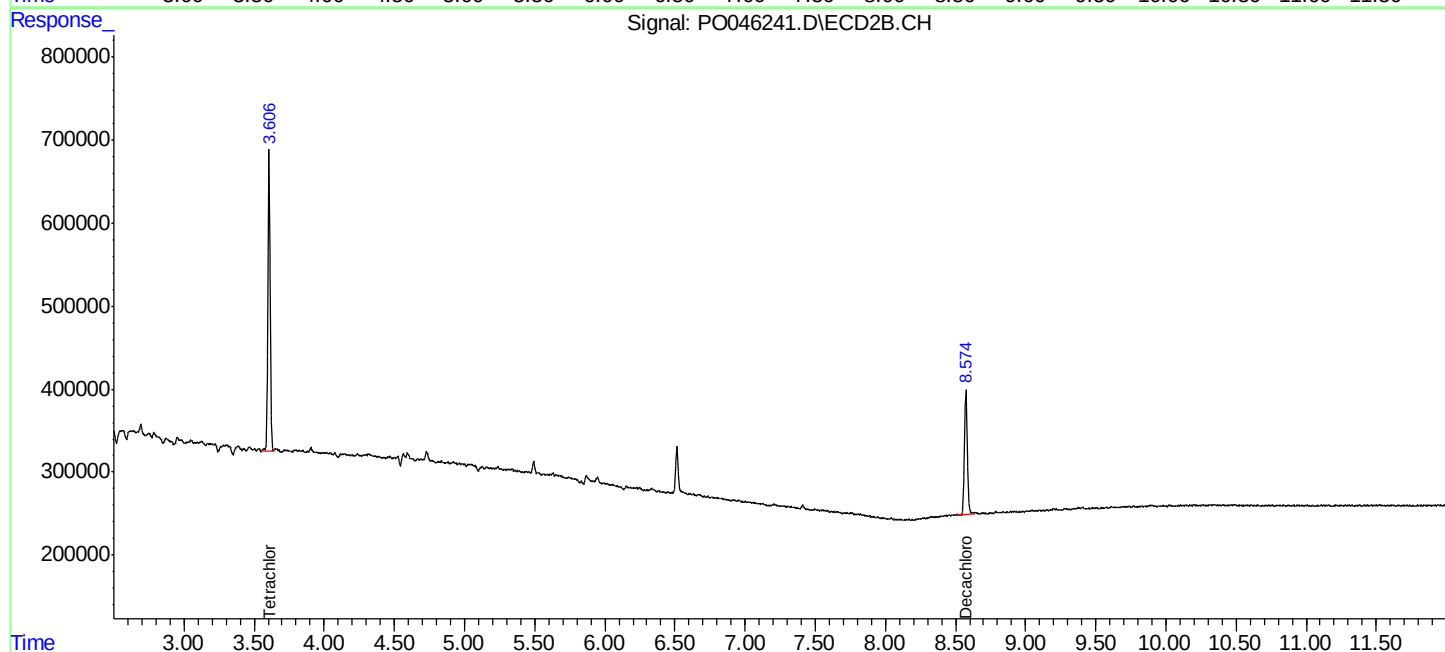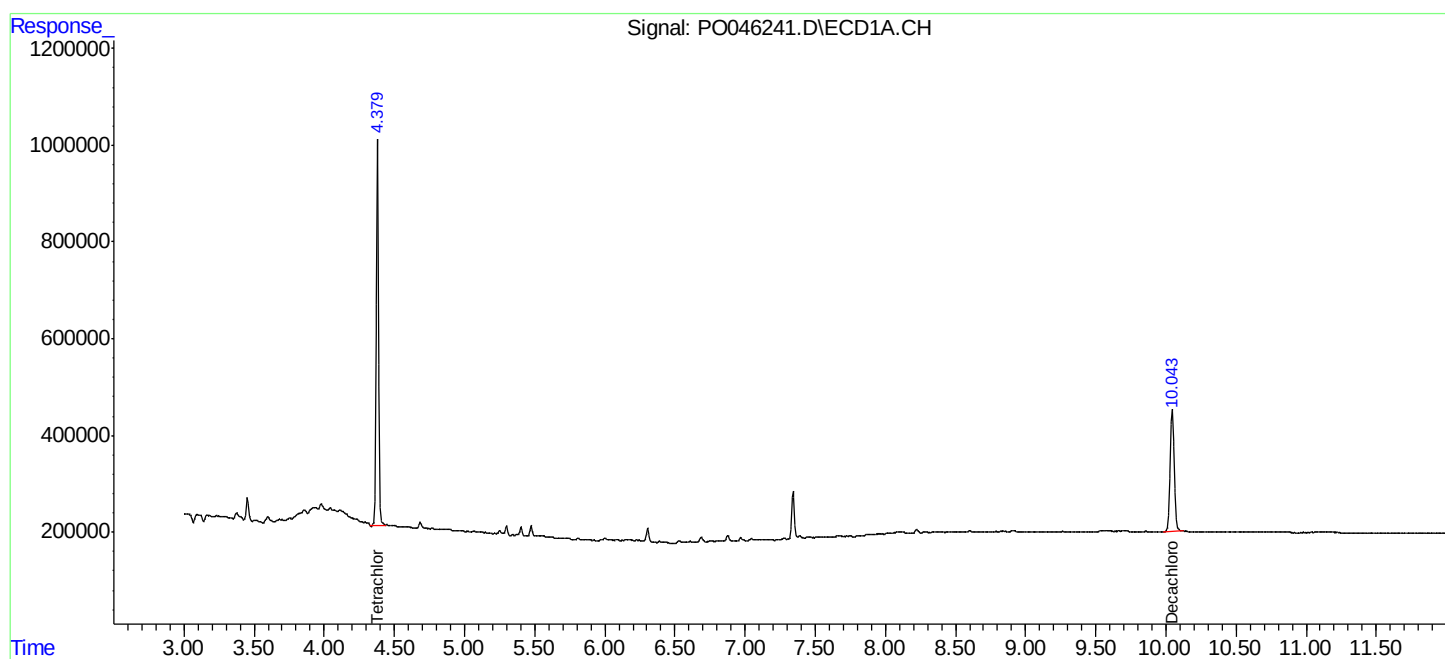


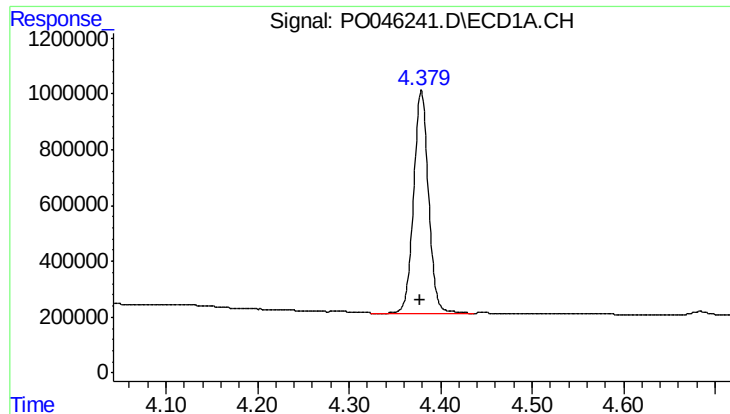

#1 Tetrachloro-m-xylene


R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 9023823
Conc: 15.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

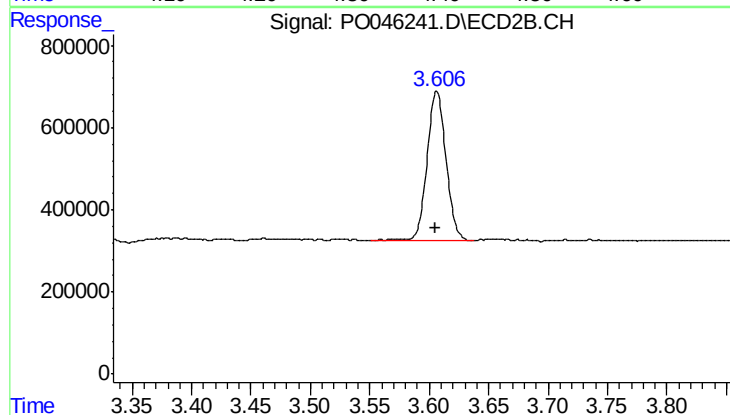


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 4049324
Conc: 16.49 ng/ml

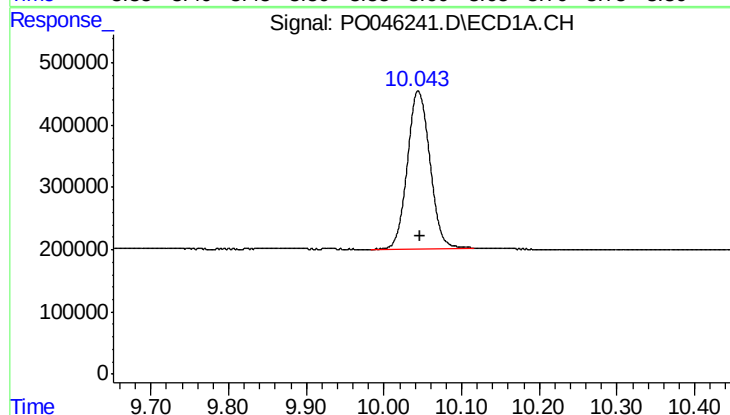

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.002 min
Response: 5143673
Conc: 11.36 ng/ml

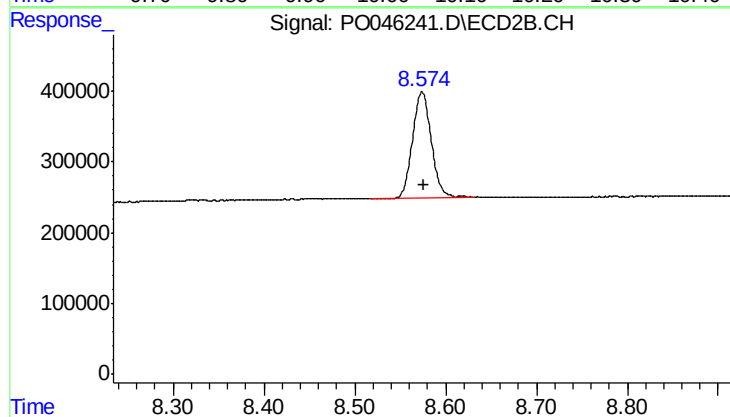

#2 Decachlorobiphenyl

R.T.: 8.574 min
Delta R.T.: -0.002 min
Response: 2144429
Conc: 13.04 ng/ml