

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062519\
 Data File : P0057432.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2019 15:17
 Operator : SM/SJ
 Sample : K3487-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-048RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:55:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.235	3.555	617945	543385	15.731	15.453
2)	SA Decachlor...	9.787	8.476	579557	391816	10.306	10.474
Target Compounds							
20)	L4 AR-1242-5	6.244	5.434	837448	421510	645.398	420.895 #
24)	L5 AR-1248-4	6.244	0.000	837448	0	357.296	N.D. #
25)	L5 AR-1248-5	6.244	5.434	837448	421510	372.932	272.546 #
26)	L6 AR-1254-1	6.244	5.434	837448	421510	429.955	198.198 #
27)	L6 AR-1254-2	0.000	5.624	0	81348	N.D.	43.706 #
28)	L6 AR-1254-3	6.839	0.000	208197	0	62.974	N.D. #
32)	L7 AR-1260-2	0.000	6.265	0	150803	N.D.	54.965 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062519\
Data File : P0057432.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2019 15:17
Operator : SM/SJ
Sample : K3487-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:55:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

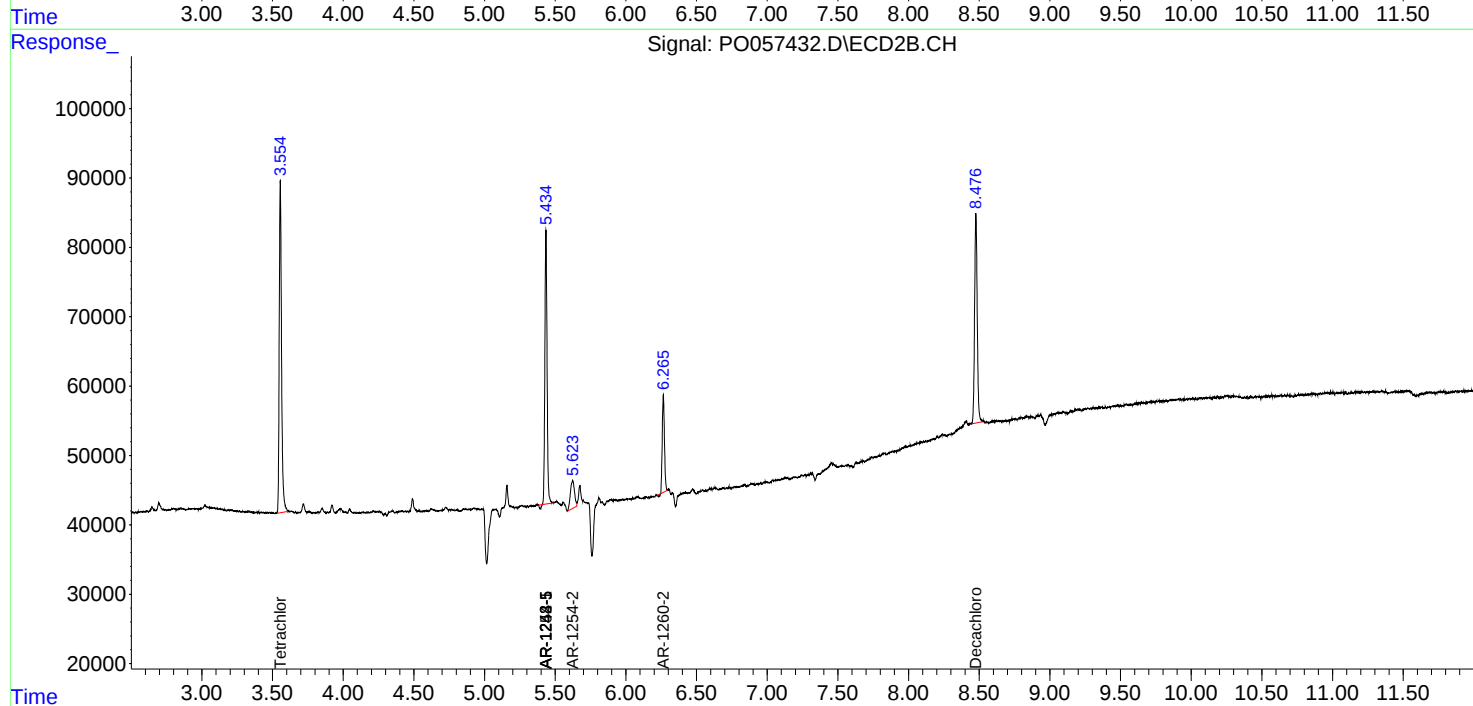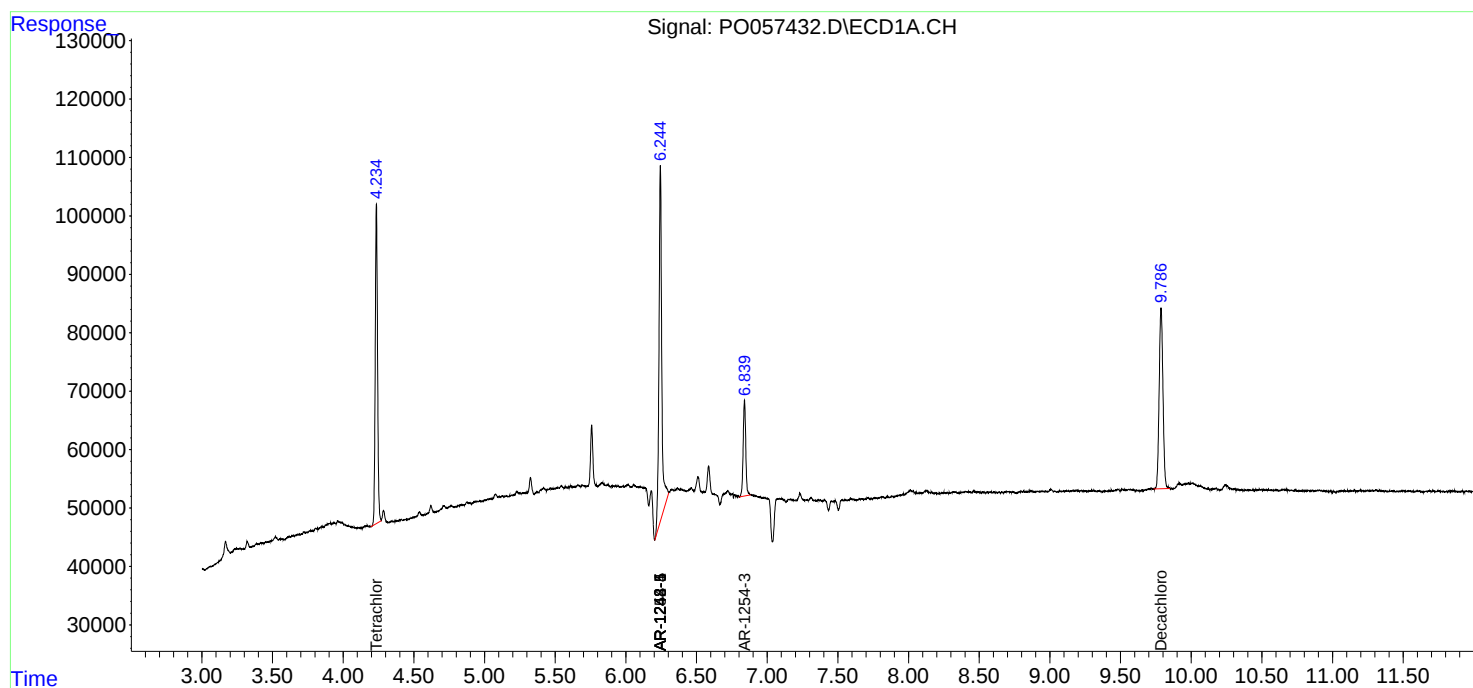


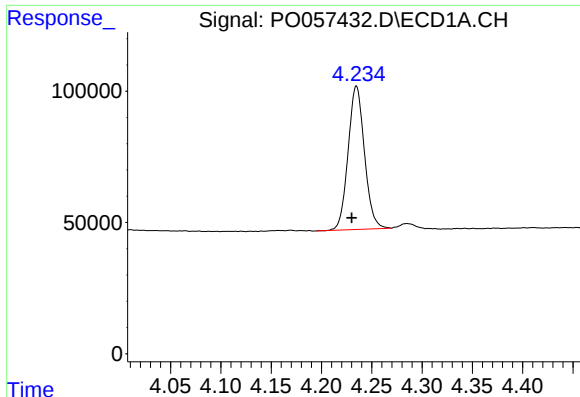

#1 Tetrachloro-m-xylene


R.T.: 4.235 min
Delta R.T.: 0.005 min
Response: 617945
Conc: 15.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048RE

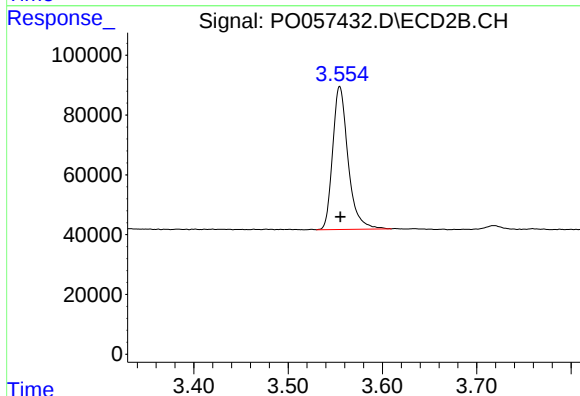


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 543385
Conc: 15.45 ng/ml

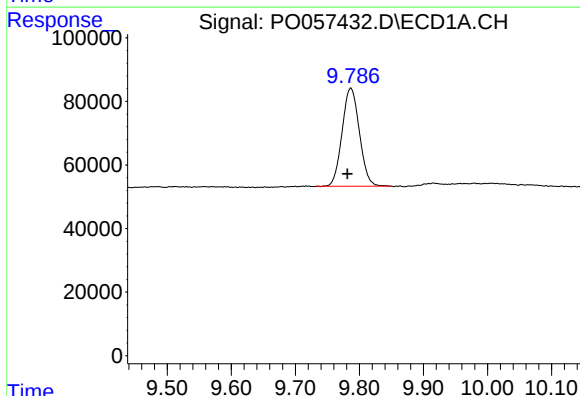


#2 Decachlorobiphenyl

R.T.: 9.787 min
Delta R.T.: 0.005 min
Response: 579557
Conc: 10.31 ng/ml

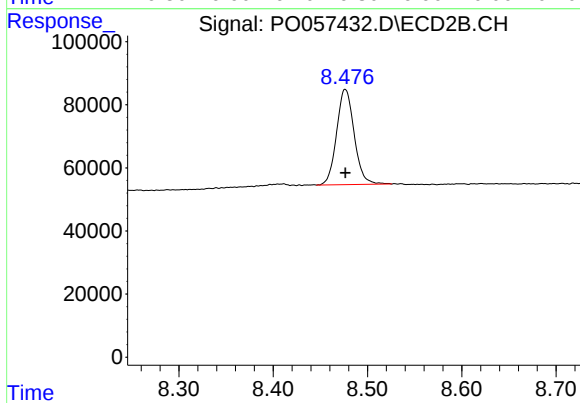

#2 Decachlorobiphenyl


R.T.: 8.476 min
Delta R.T.: 0.000 min
Response: 391816
Conc: 10.47 ng/ml

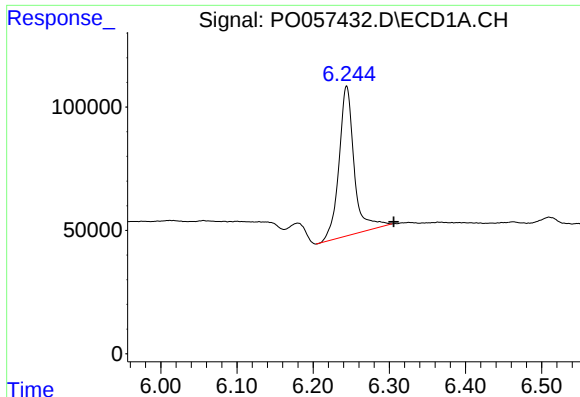

#20 AR-1242-5


R.T.: 6.244 min
Delta R.T.: -0.062 min
Response: 837448
Conc: 645.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048RE

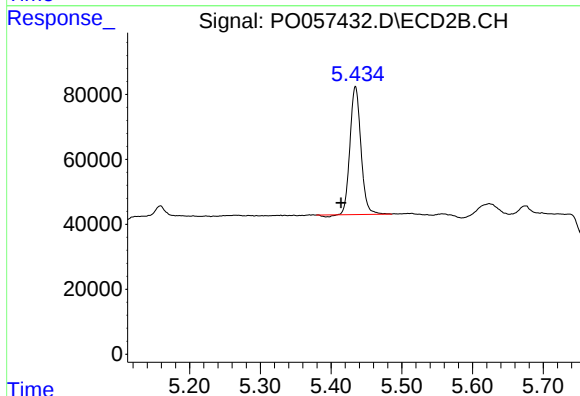


#20 AR-1242-5

R.T.: 5.434 min
Delta R.T.: 0.020 min
Response: 421510
Conc: 420.89 ng/ml

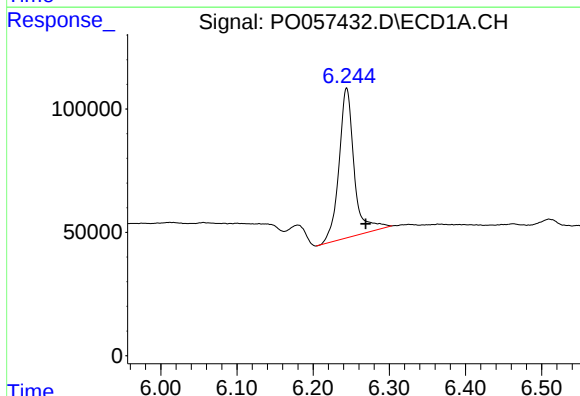


#24 AR-1248-4

R.T.: 6.244 min
Delta R.T.: -0.025 min
Response: 837448
Conc: 357.30 ng/ml

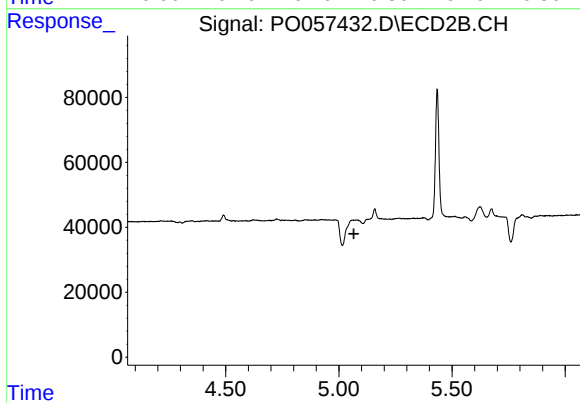

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

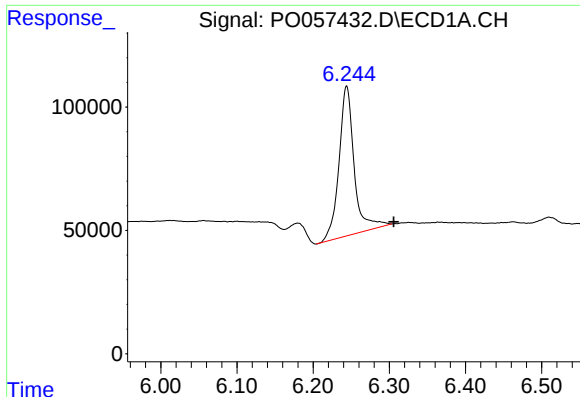

#25 AR-1248-5


R.T.: 6.244 min
Delta R.T.: -0.062 min
Response: 837448
Conc: 372.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048RE

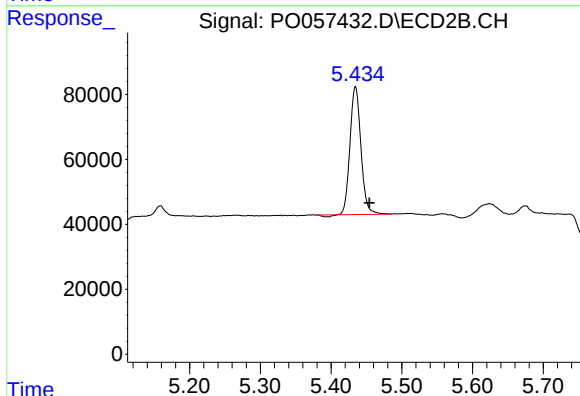


#25 AR-1248-5

R.T.: 5.434 min
Delta R.T.: -0.019 min
Response: 421510
Conc: 272.55 ng/ml

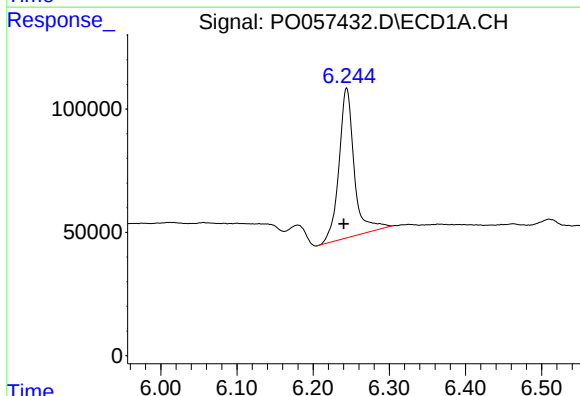


#26 AR-1254-1

R.T.: 6.244 min
Delta R.T.: 0.004 min
Response: 837448
Conc: 429.96 ng/ml

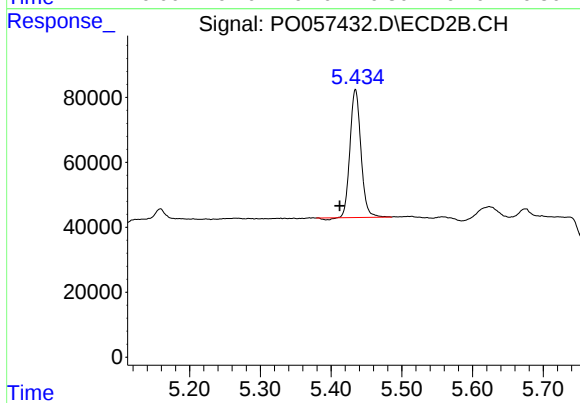

#26 AR-1254-1


R.T.: 5.434 min
Delta R.T.: 0.022 min
Response: 421510
Conc: 198.20 ng/ml

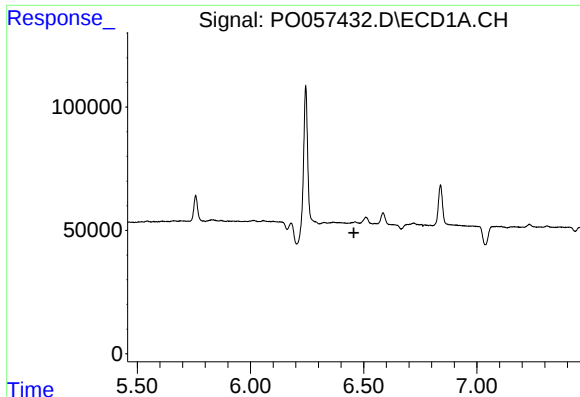

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048RE

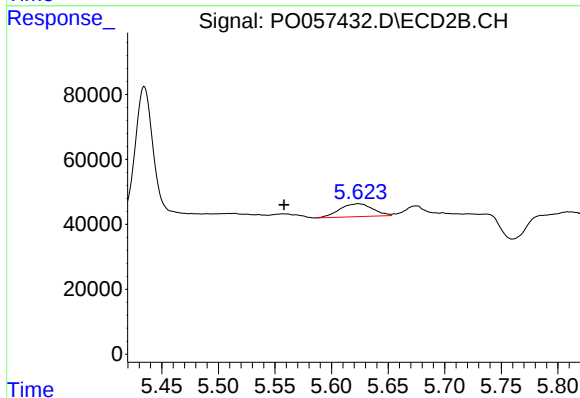


#27 AR-1254-2

R.T.: 5.624 min
Delta R.T.: 0.066 min
Response: 81348
Conc: 43.71 ng/ml

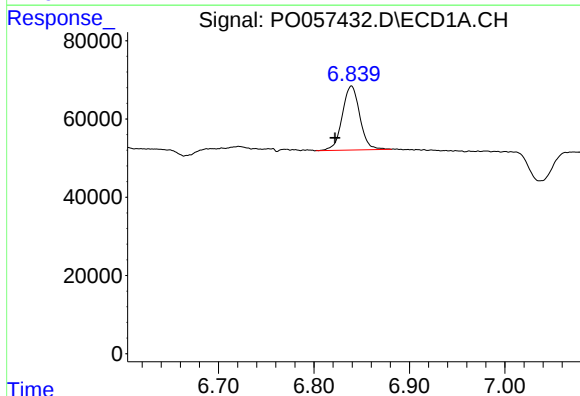


#28 AR-1254-3

R.T.: 6.839 min
Delta R.T.: 0.017 min
Response: 208197
Conc: 62.97 ng/ml

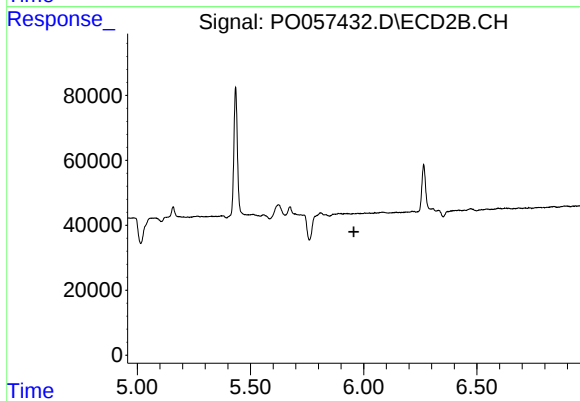

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 5.957 min
Response: 0
Conc: N.D.

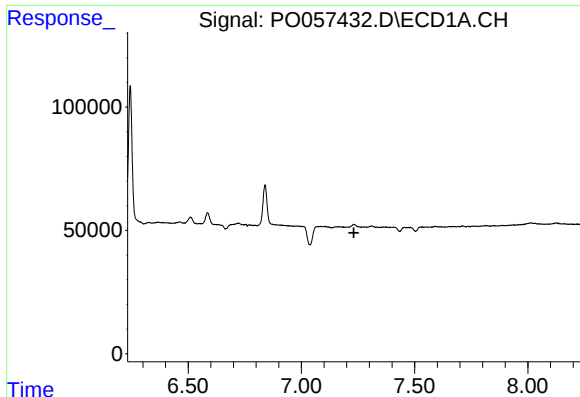

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048RE

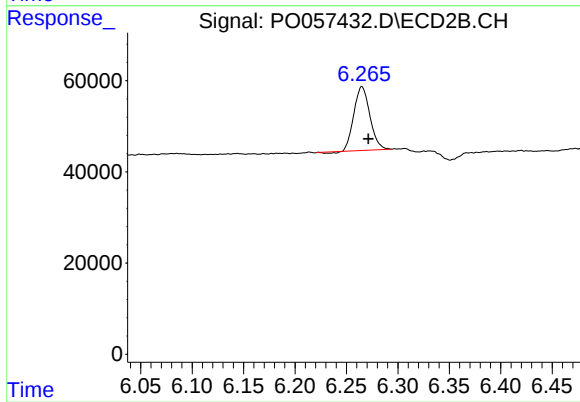

#32 AR-1260-2

R.T.: 6.265 min
Delta R.T.: -0.006 min
Response: 150803
Conc: 54.96 ng/ml