

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062519\
Data File : P0057446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2019 19:29
Operator : SM/SJ
Sample : K3499-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TWP-B-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:58:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.229	3.557	708847	657493	18.045	18.698
2) SA Decachlor...	9.777	8.474	889174	599342	15.812	16.022

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062519\
Data File : P0057446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2019 19:29
Operator : SM/SJ
Sample : K3499-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TWP-B-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:58:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

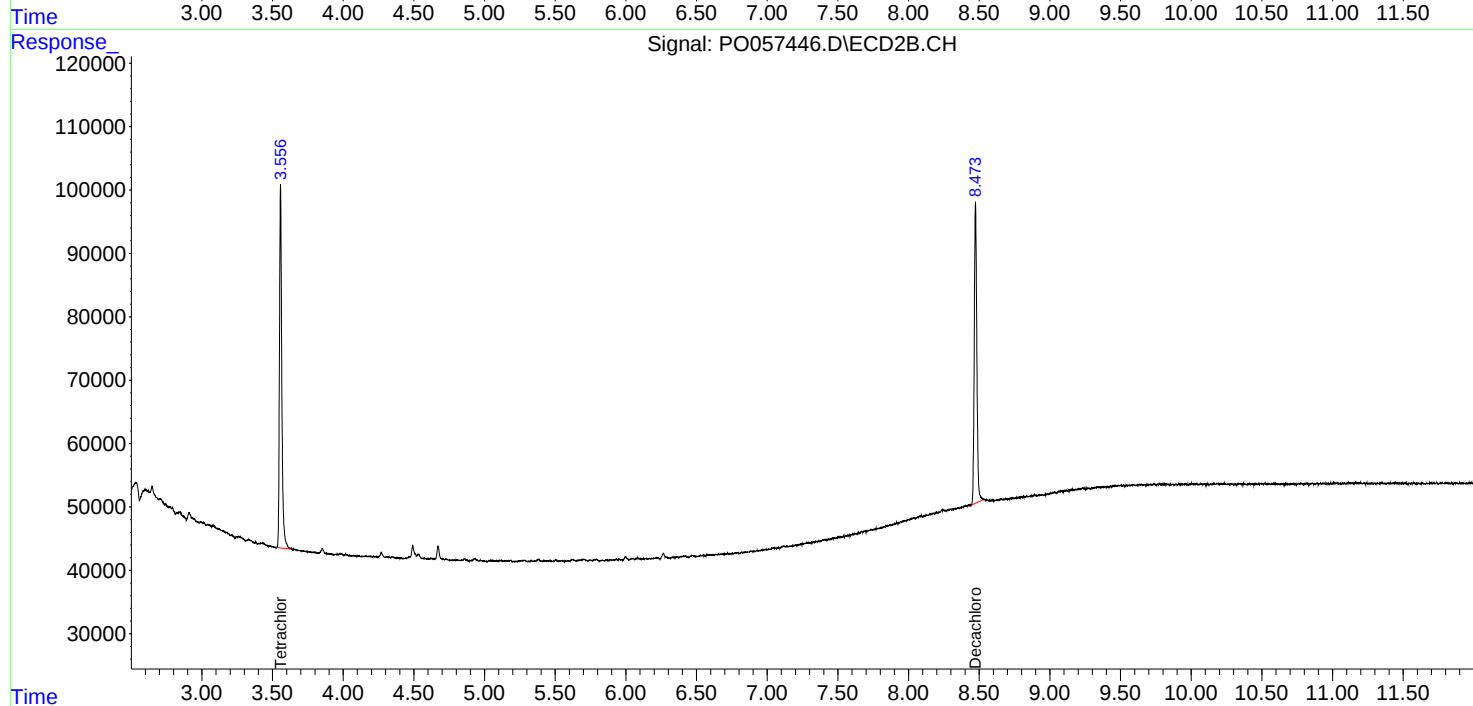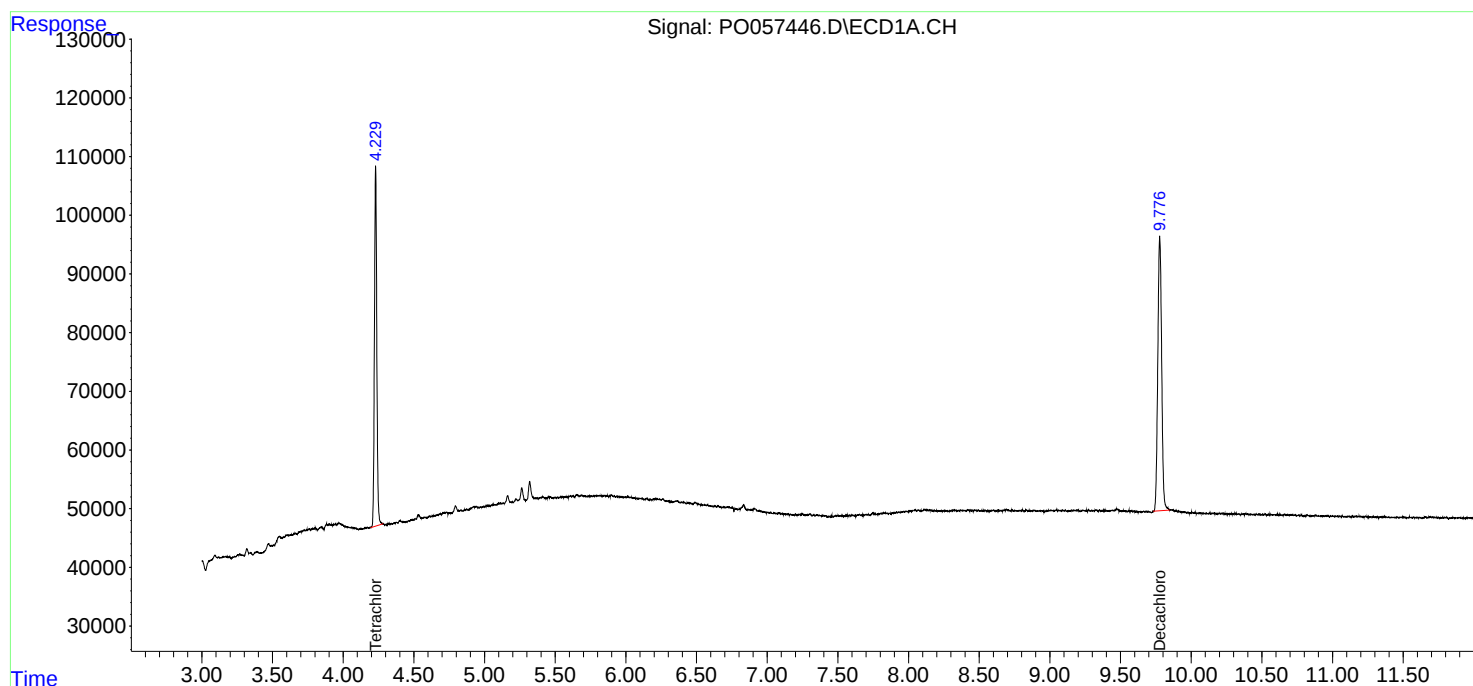


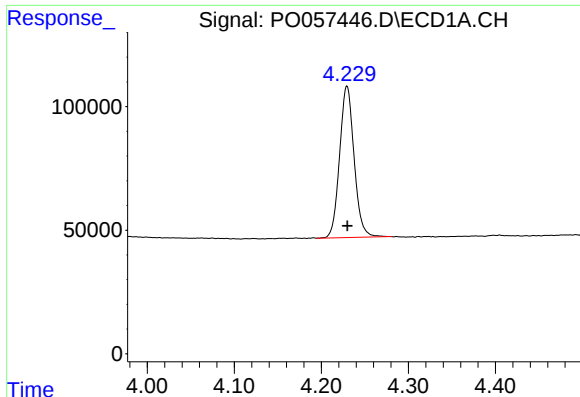

#1 Tetrachloro-m-xylene


R.T.: 4.229 min
Delta R.T.: 0.000 min
Response: 708847
Conc: 18.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TWP-B-6

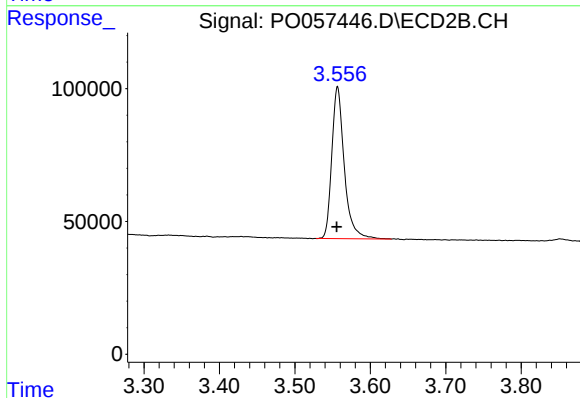


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.001 min
Response: 657493
Conc: 18.70 ng/ml

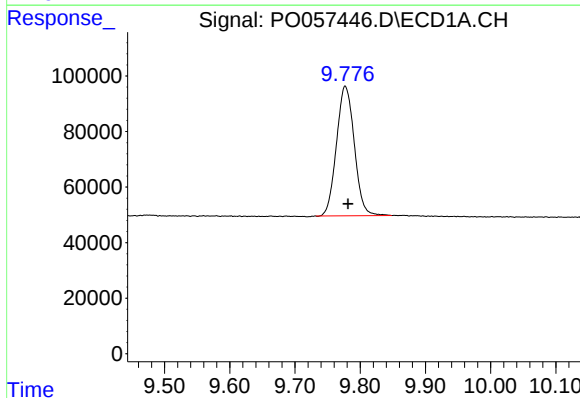

#2 Decachlorobiphenyl

R.T.: 9.777 min
Delta R.T.: -0.004 min
Response: 889174
Conc: 15.81 ng/ml

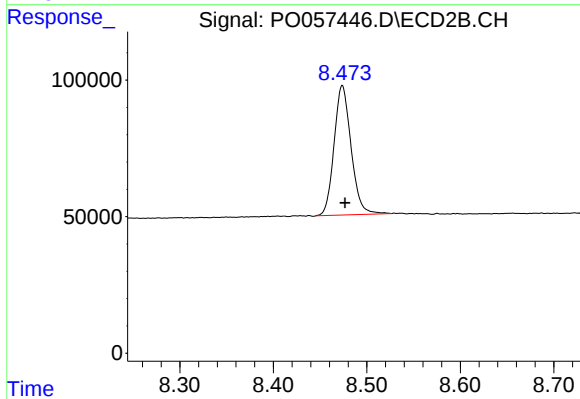

#2 Decachlorobiphenyl

R.T.: 8.474 min
Delta R.T.: -0.003 min
Response: 599342
Conc: 16.02 ng/ml