

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062519\
 Data File : P0057428.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2019 13:43
 Operator : SM/SJ
 Sample : K3429-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-002-IDW/GW-20190617

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 14:02:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.228	3.554	646819	562422	16.466	15.995
2)	SA Decachlor...	9.778	8.474	1011559	670745	17.989	17.931

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062519\
Data File : P0057428.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2019 13:43
Operator : SM/SJ
Sample : K3429-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-002-IDW/GW-20190617

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 14:02:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

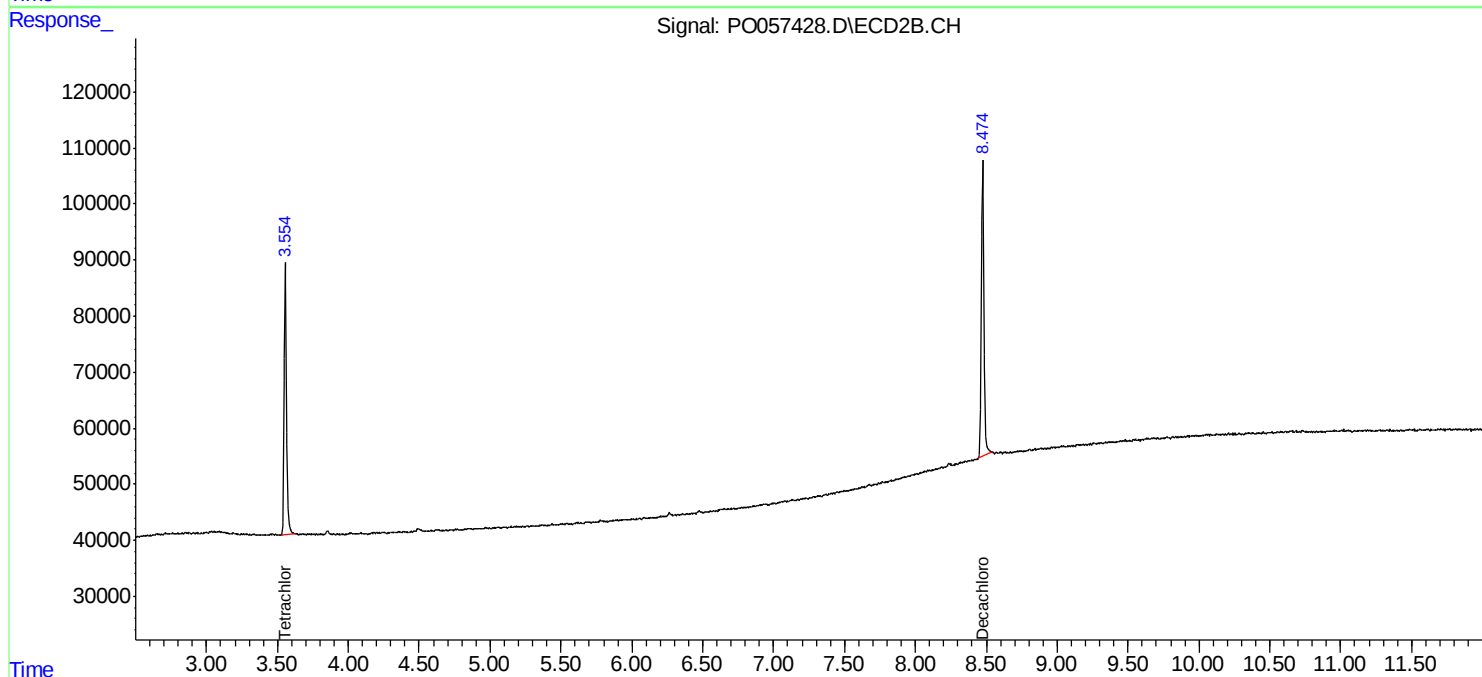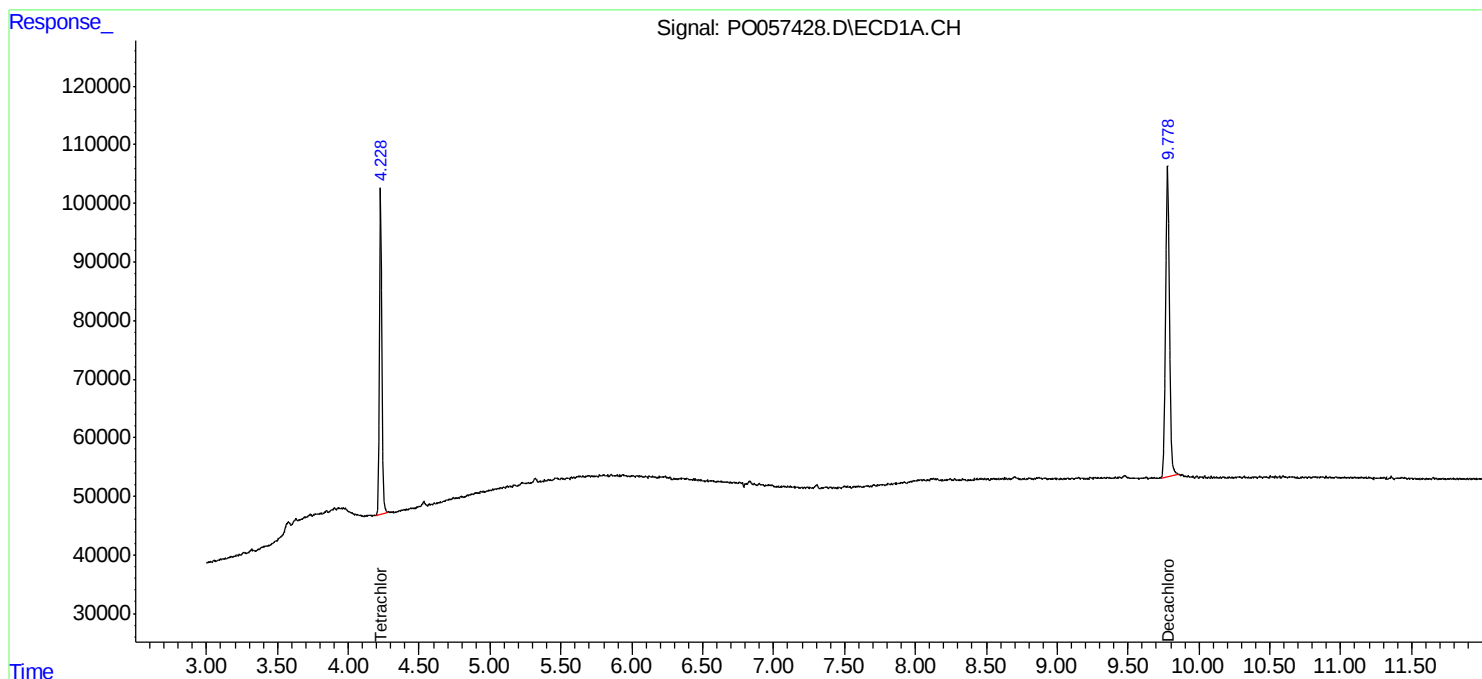


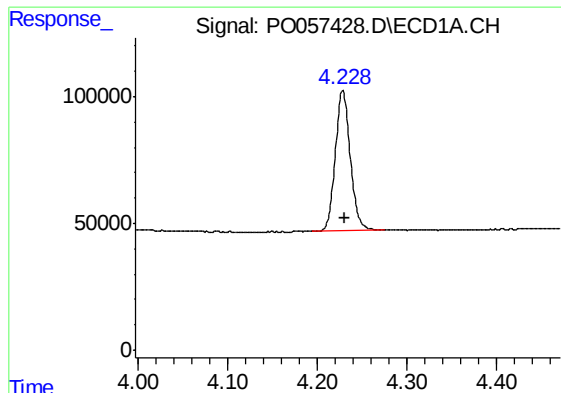

#1 Tetrachloro-m-xylene


R.T.: 4.228 min
Delta R.T.: -0.002 min
Response: 646819
Conc: 16.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-002-IDW/GW-20190617

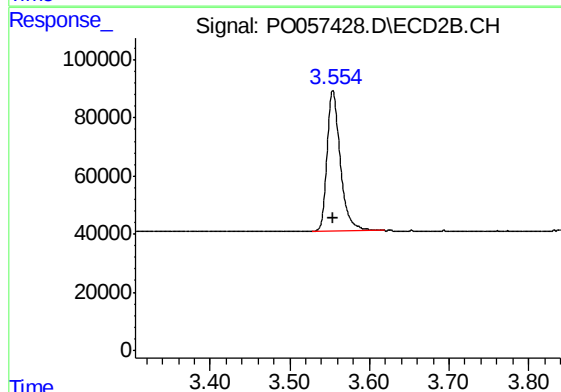


#1 Tetrachloro-m-xylene

R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 562422
Conc: 15.99 ng/ml

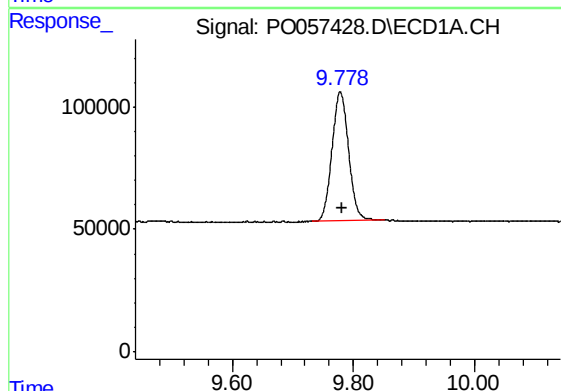

#2 Decachlorobiphenyl

R.T.: 9.778 min
Delta R.T.: -0.003 min
Response: 1011559
Conc: 17.99 ng/ml

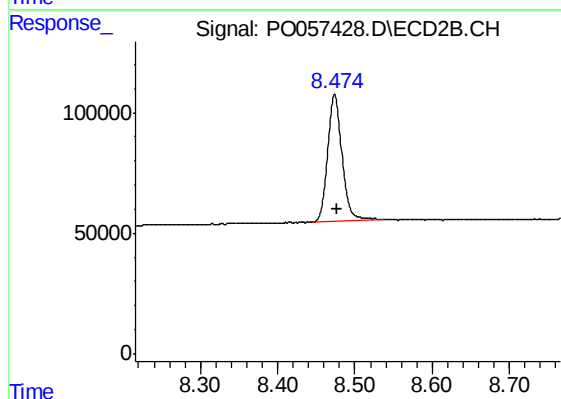

#2 Decachlorobiphenyl

R.T.: 8.474 min
Delta R.T.: -0.003 min
Response: 670745
Conc: 17.93 ng/ml