

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062620\
 Data File : P0069225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2020 8:55
 Operator : DD\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Manual Integrations
 APPROVED

Ankita
 6/30/2020 1:44:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 09:11:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 26 09:08:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.563	740366	895603	25.361	25.369
2) SA Decachlor...	10.066	8.773	1303621	1316384	25.630	26.590
Target Compounds						
26) L6 AR-1254-1	6.604	5.653	371959	606571	249.560m	264.892
27) L6 AR-1254-2	6.834	5.814	604602	545928	261.884	266.920
28) L6 AR-1254-3	7.210	6.225	648415	869145	259.219	263.374
29) L6 AR-1254-4	7.507	6.466	537638	587034	258.678	263.004
30) L6 AR-1254-5	7.929	6.890	516034	806897	240.831	262.854

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062620\
Data File : PO069225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2020 8:55
Operator : DD\AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 09:11:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 26 09:08:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

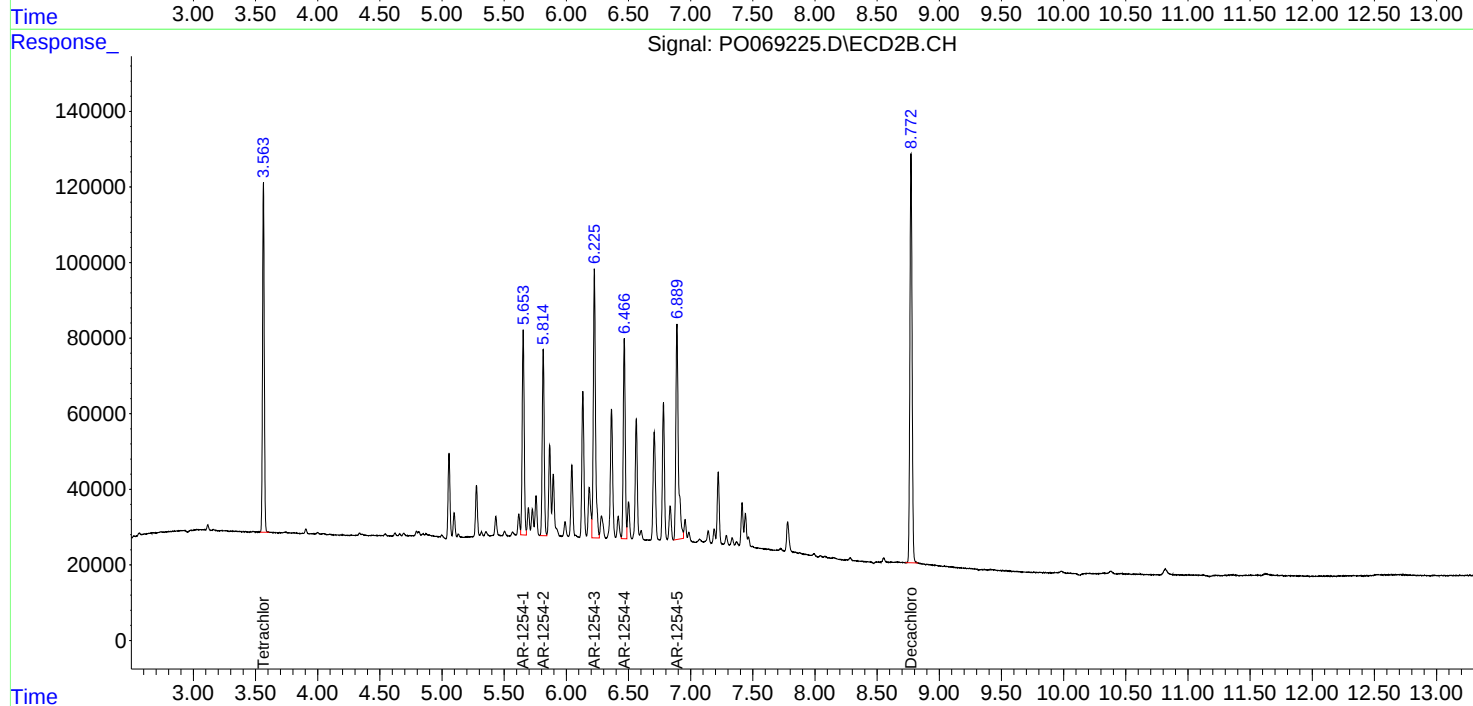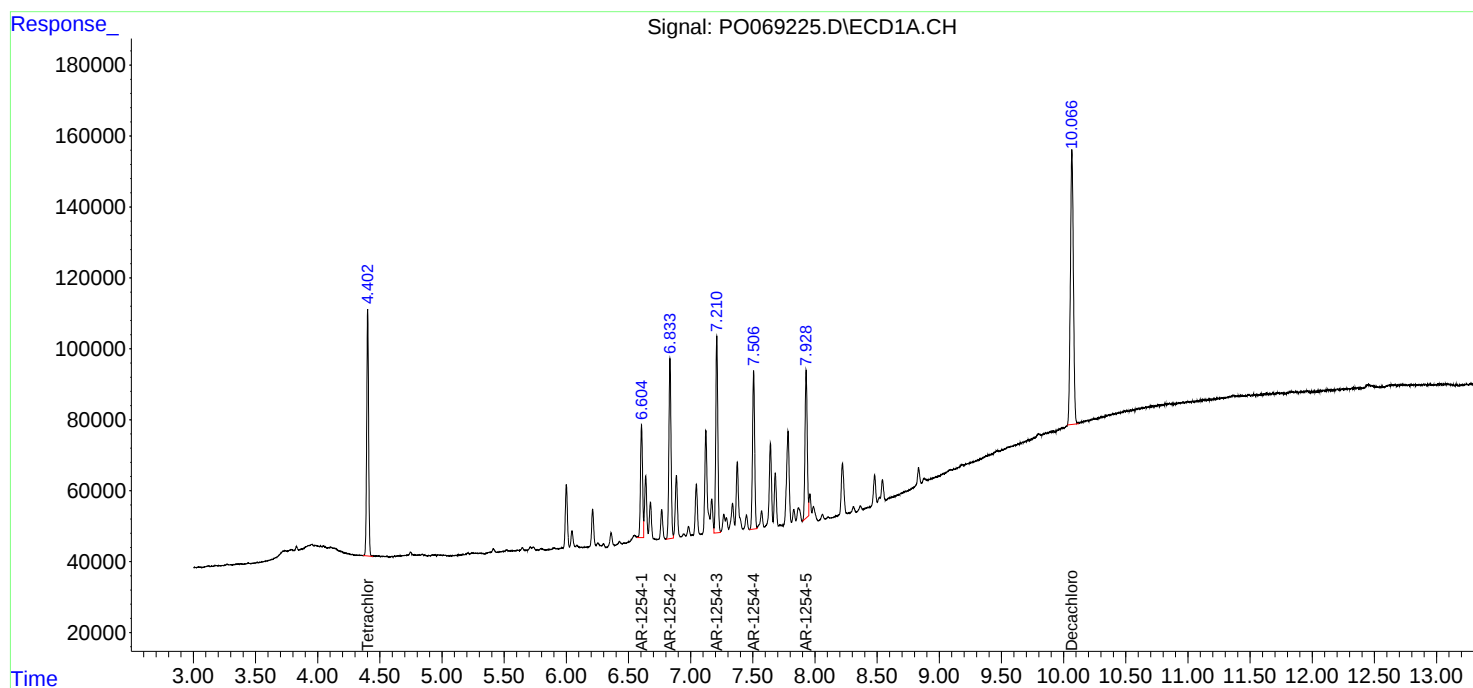

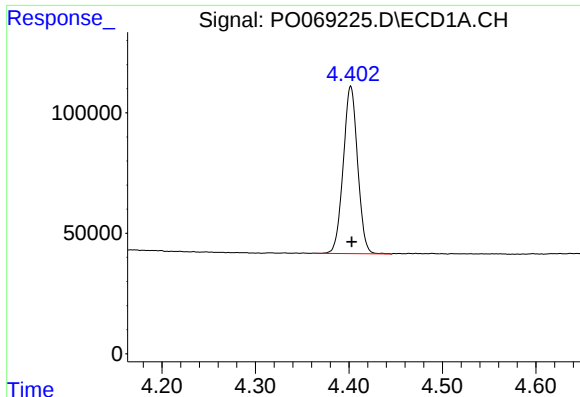


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: 0.000 min
Response: 740366
Conc: 25.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:25 PM

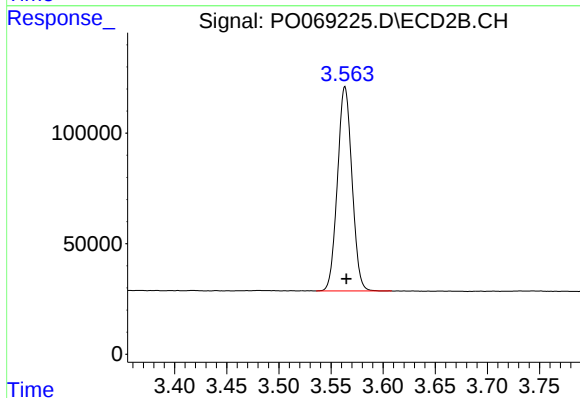


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.001 min
Response: 895603
Conc: 25.37 ng/ml

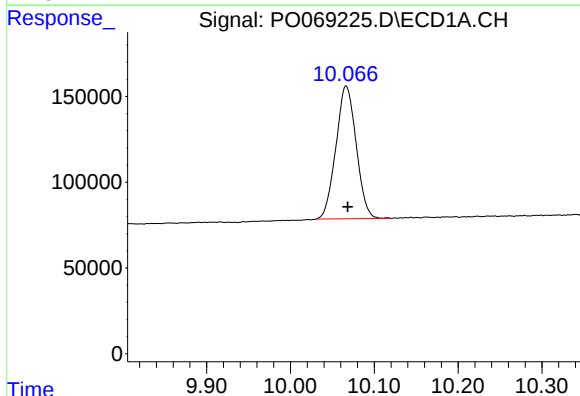


#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.002 min
Response: 1303621
Conc: 25.63 ng/ml

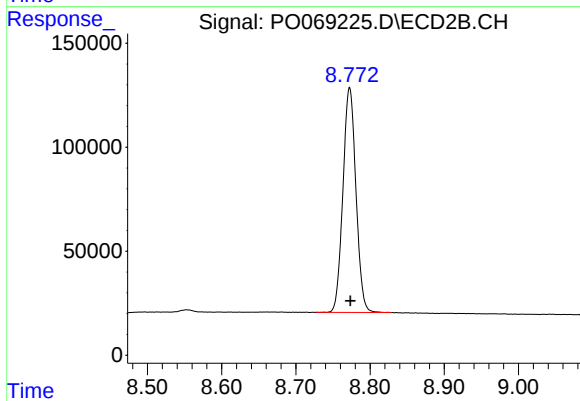

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.000 min
Response: 1316384
Conc: 26.59 ng/ml

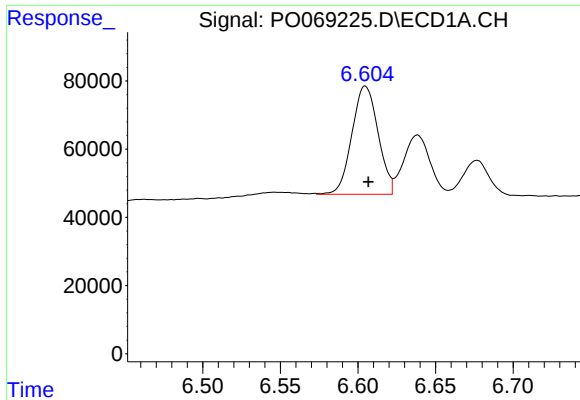


#26 AR-1254-1

R.T.: 6.604 min
Delta R.T.: -0.002 min
Response: 371959
Conc: 249.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:25 PM

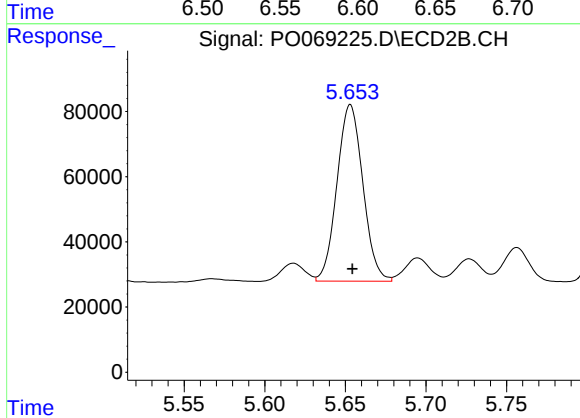


#26 AR-1254-1

R.T.: 5.653 min
Delta R.T.: -0.001 min
Response: 606571
Conc: 264.89 ng/ml

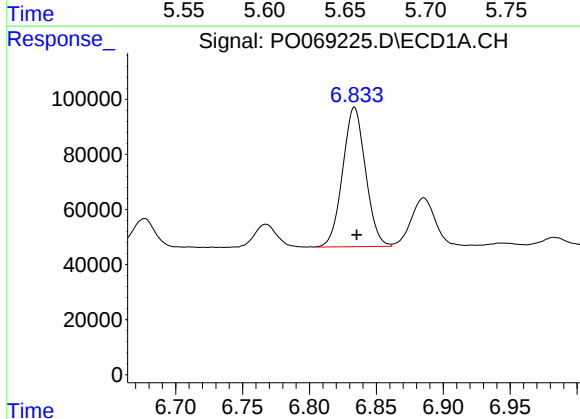


#27 AR-1254-2

R.T.: 6.834 min
Delta R.T.: -0.002 min
Response: 604602
Conc: 261.88 ng/ml

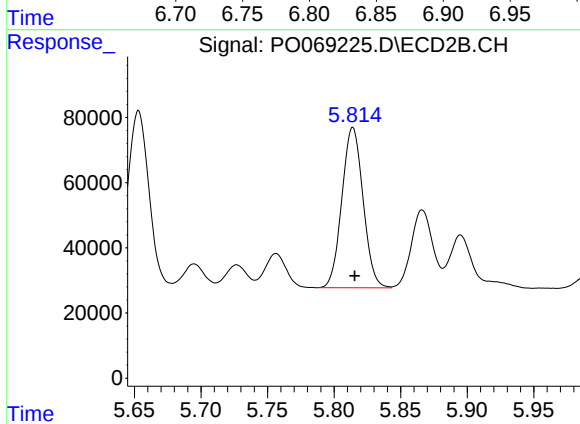

#27 AR-1254-2

R.T.: 5.814 min
Delta R.T.: -0.001 min
Response: 545928
Conc: 266.92 ng/ml

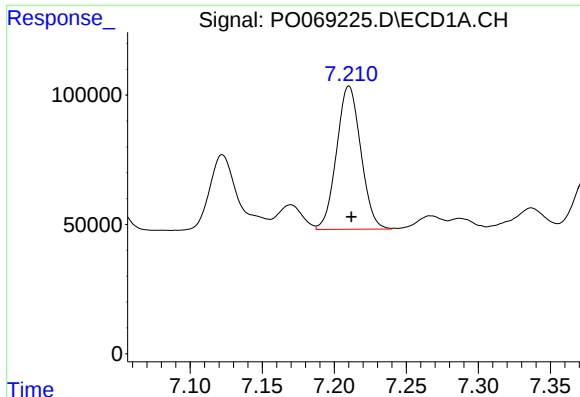


#28 AR-1254-3

R.T.: 7.210 min
Delta R.T.: -0.002 min
Response: 648415
Conc: 259.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:25 PM

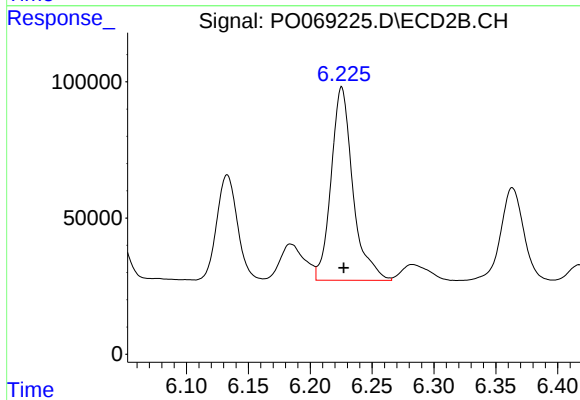


#28 AR-1254-3

R.T.: 6.225 min
Delta R.T.: -0.002 min
Response: 869145
Conc: 263.37 ng/ml

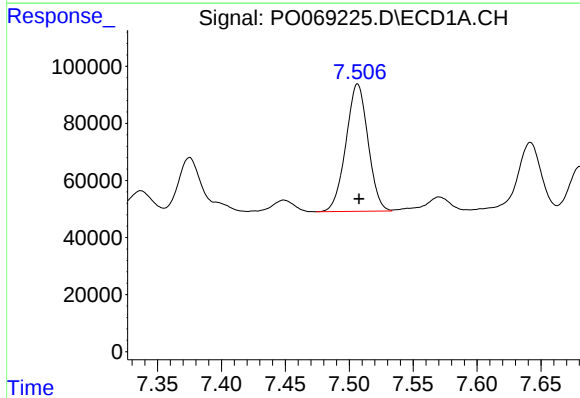


#29 AR-1254-4

R.T.: 7.507 min
Delta R.T.: -0.001 min
Response: 537638
Conc: 258.68 ng/ml

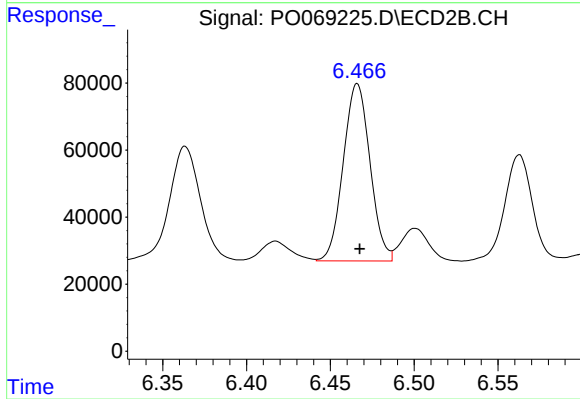

#29 AR-1254-4

R.T.: 6.466 min
Delta R.T.: -0.001 min
Response: 587034
Conc: 263.00 ng/ml

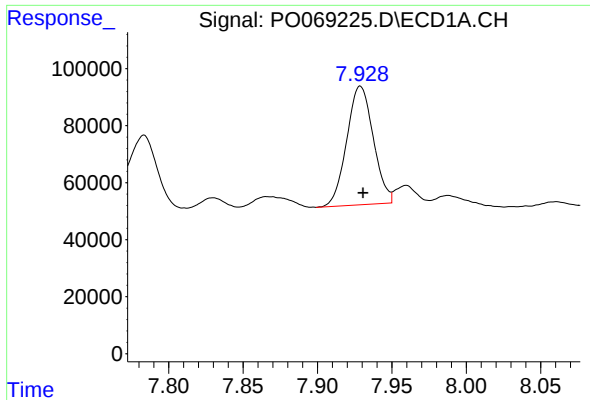


#30 AR-1254-5

R.T.: 7.929 min
Delta R.T.: -0.002 min
Response: 516034
Conc: 240.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:25 PM

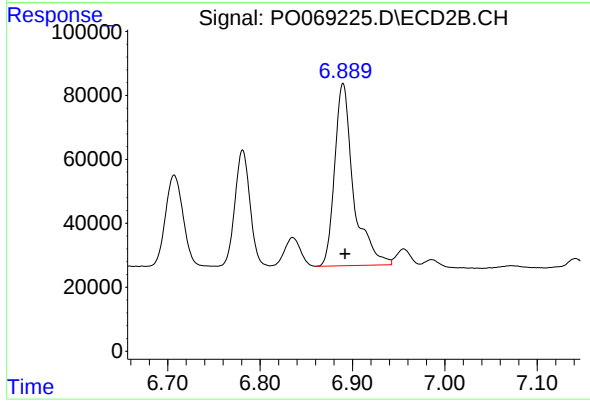

#30 AR-1254-5

R.T.: 6.890 min
Delta R.T.: -0.002 min
Response: 806897
Conc: 262.85 ng/ml