

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062620\
 Data File : P0069226.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2020 9:12
 Operator : DD\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 6/30/2020 1:44:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 09:29:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 26 09:08:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.563	168415	199234	5.769	5.643
2) SA Decachlor...	10.066	8.772	290044	336113	5.702	6.789
Target Compounds						
26) L6 AR-1254-1	6.604	5.653	79263	137530	53.180m	60.060
27) L6 AR-1254-2	6.833	5.814	144224	130508	62.471	63.809
28) L6 AR-1254-3	7.209	6.226	147976	201498	59.157	61.059
29) L6 AR-1254-4	7.505	6.466	124199	129646	59.757	58.085
30) L6 AR-1254-5	7.929	6.890	105109	184285	49.054	60.033

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062620\
Data File : PO069226.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2020 9:12
Operator : DD\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 09:29:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 26 09:08:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

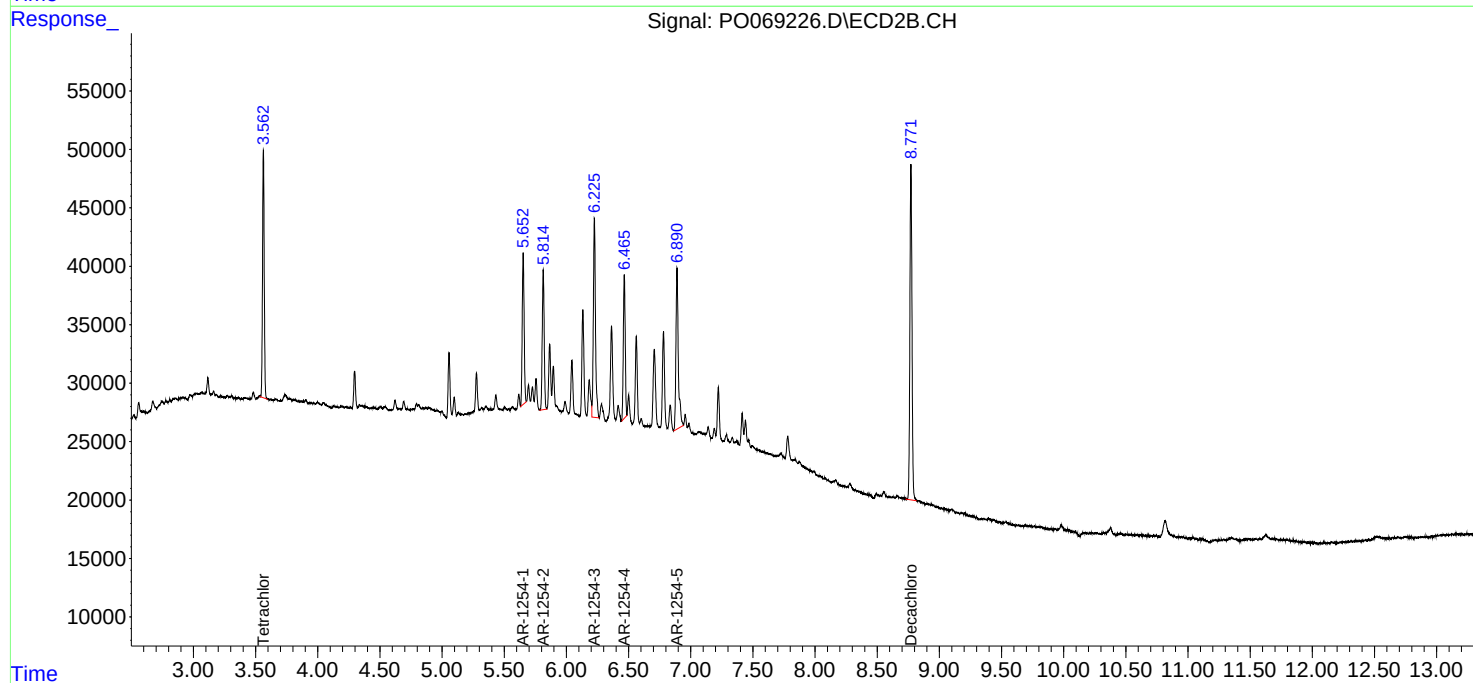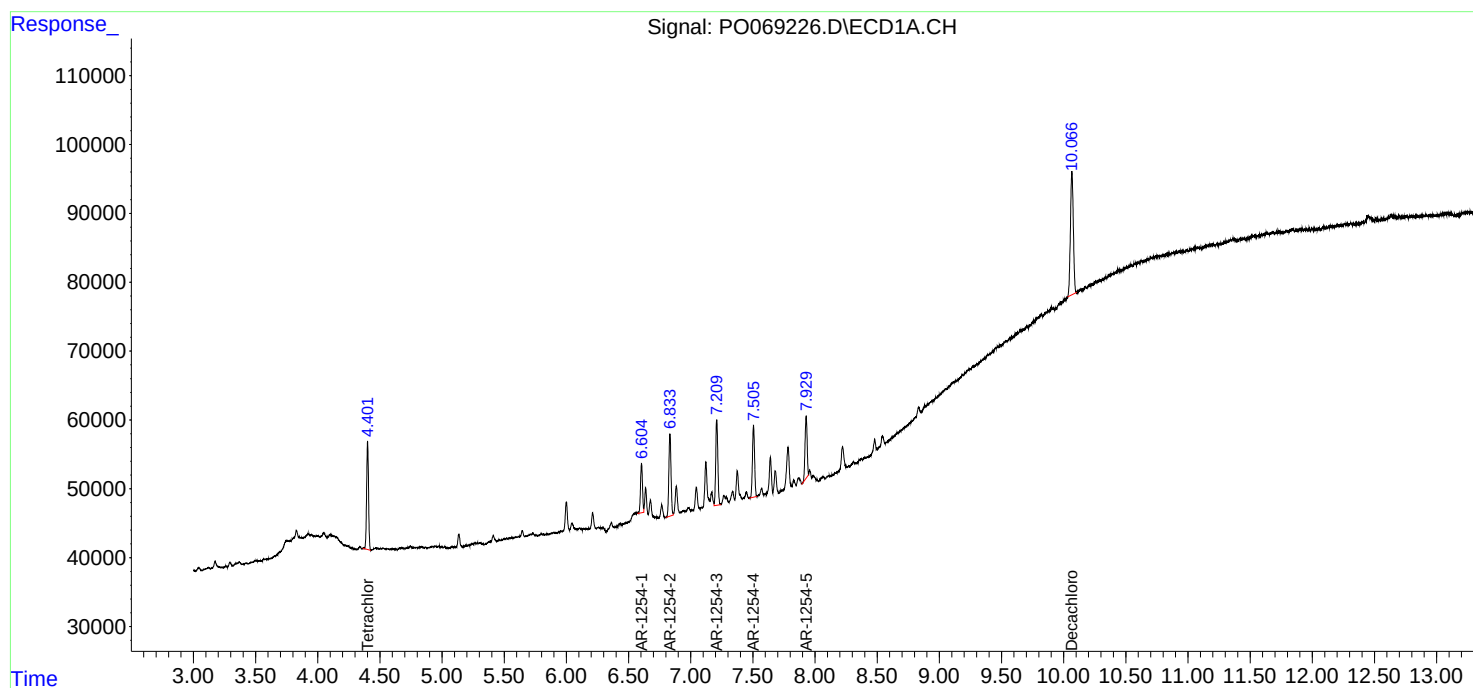

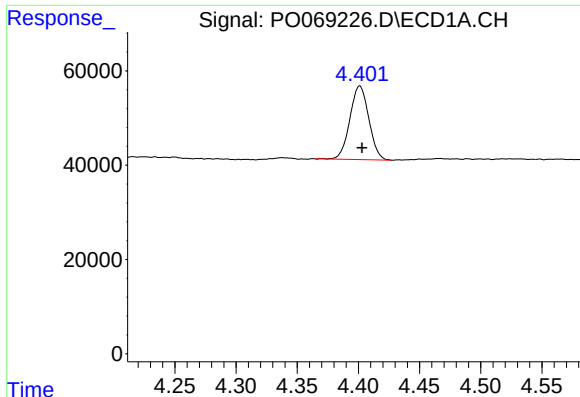


#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.002 min
Response: 168415
Conc: 5.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:30 PM

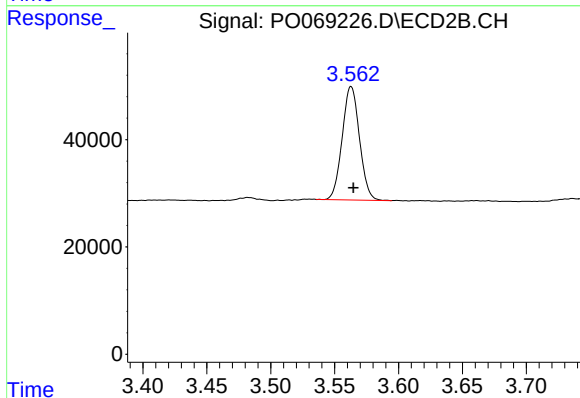


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.002 min
Response: 199234
Conc: 5.64 ng/ml

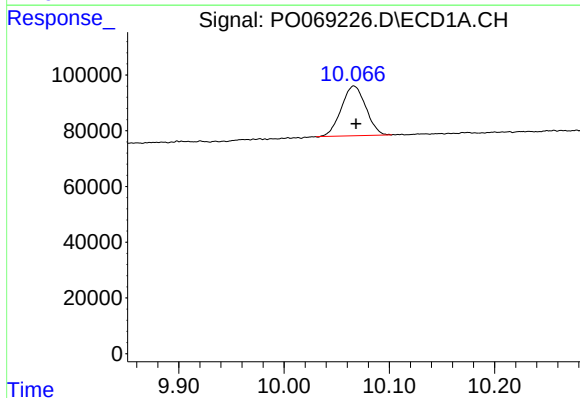


#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.002 min
Response: 290044
Conc: 5.70 ng/ml

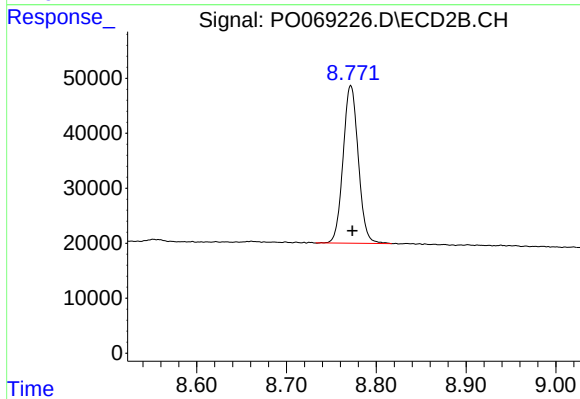

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: -0.002 min
Response: 336113
Conc: 6.79 ng/ml

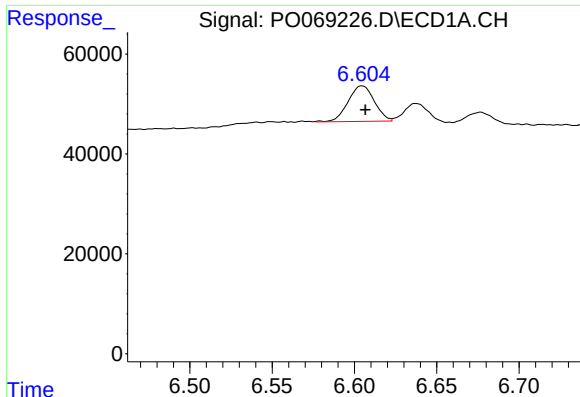


#26 AR-1254-1

R.T.: 6.604 min
Delta R.T.: -0.003 min
Response: 79263
Conc: 53.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:30 PM

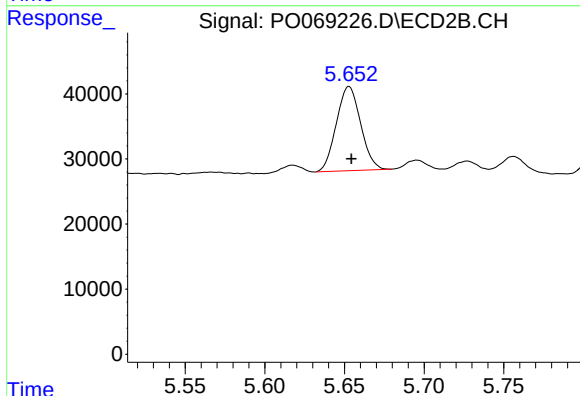


#26 AR-1254-1

R.T.: 5.653 min
Delta R.T.: -0.001 min
Response: 137530
Conc: 60.06 ng/ml

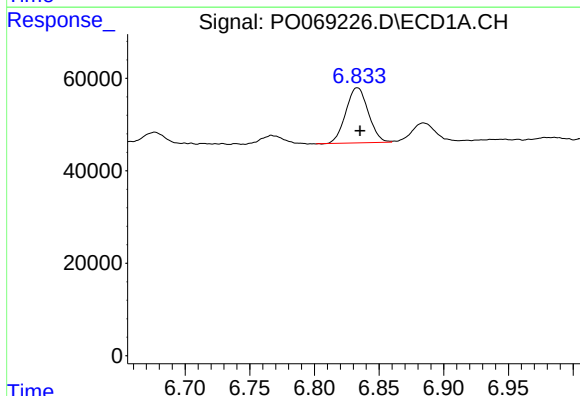


#27 AR-1254-2

R.T.: 6.833 min
Delta R.T.: -0.002 min
Response: 144224
Conc: 62.47 ng/ml

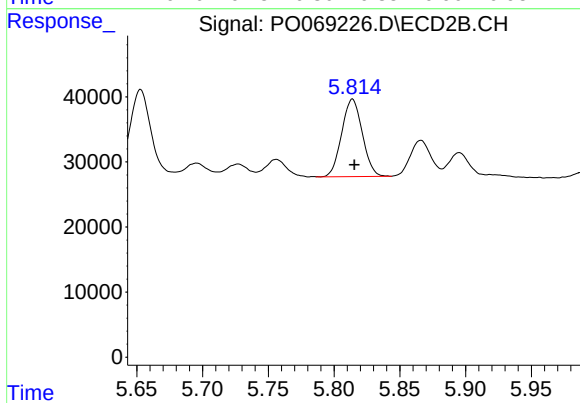

#27 AR-1254-2

R.T.: 5.814 min
Delta R.T.: -0.001 min
Response: 130508
Conc: 63.81 ng/ml

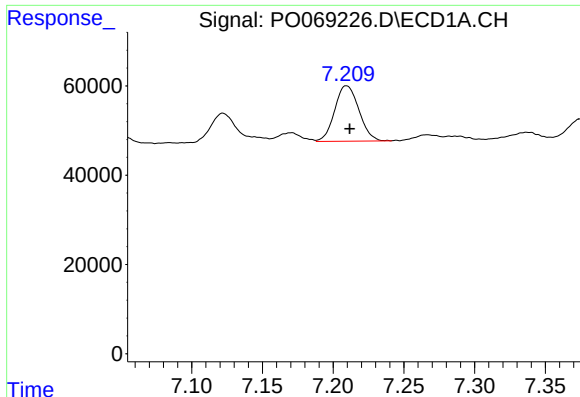


#28 AR-1254-3

R.T.: 7.209 min
Delta R.T.: -0.002 min
Response: 147976
Conc: 59.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:30 PM

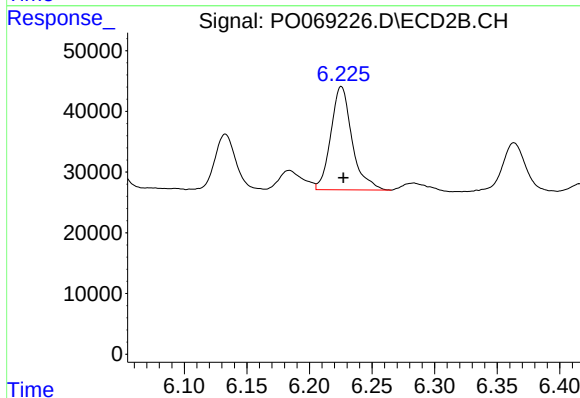


#28 AR-1254-3

R.T.: 6.226 min
Delta R.T.: -0.001 min
Response: 201498
Conc: 61.06 ng/ml

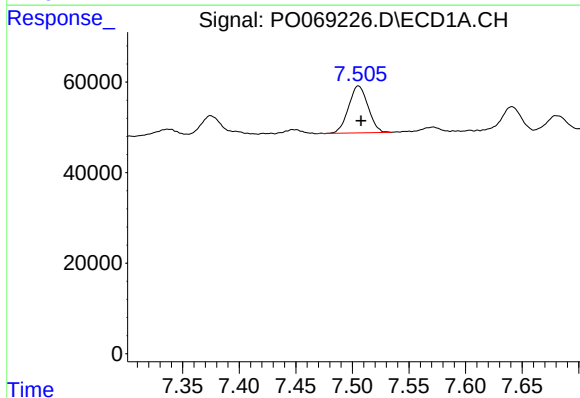


#29 AR-1254-4

R.T.: 7.505 min
Delta R.T.: -0.002 min
Response: 124199
Conc: 59.76 ng/ml

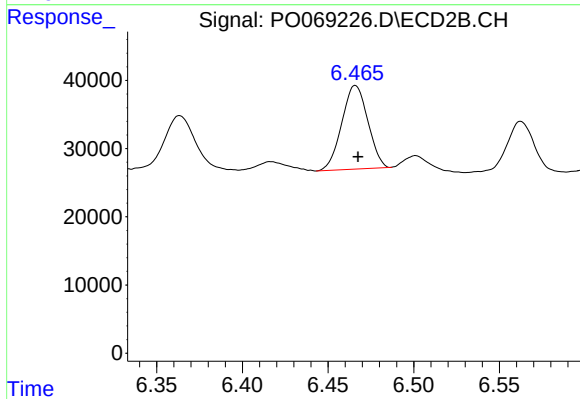

#29 AR-1254-4

R.T.: 6.466 min
Delta R.T.: -0.001 min
Response: 129646
Conc: 58.08 ng/ml

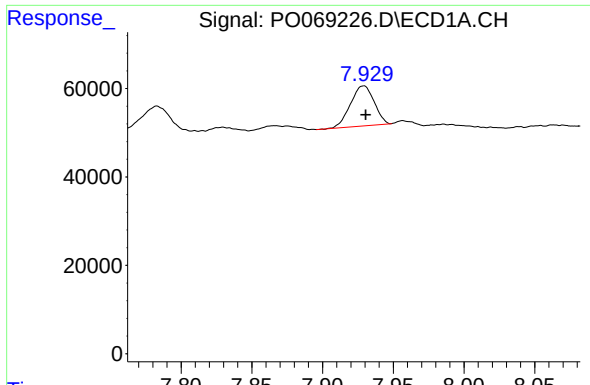


#30 AR-1254-5

R.T.: 7.929 min
Delta R.T.: -0.002 min
Response: 105109
Conc: 49.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
6/30/2020 1:44:30 PM

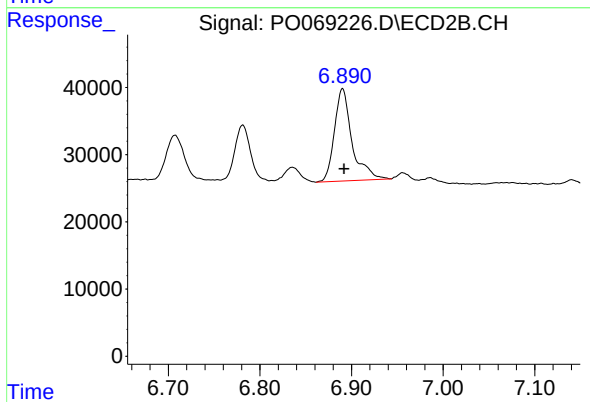

#30 AR-1254-5

R.T.: 6.890 min
Delta R.T.: -0.002 min
Response: 184285
Conc: 60.03 ng/ml