

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062620\
 Data File : P0069259.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2020 20:03
 Operator : DD\AJ
 Sample : L3130-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WOOSPK-016-0004

Manual Integrations
 APPROVED

Ankita
 6/30/2020 1:45:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 01:30:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 26 09:50:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.565	729140	852800	24.647	22.157
2) SA Decachlor...	10.068	8.775	1126303	1007295	23.714	18.504m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062620\
Data File : P0069259.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2020 20:03
Operator : DD\AJ
Sample : L3130-01
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WOOSPK-016-0004


Manual Integrations
APPROVED

Ankita
6/30/2020 1:45:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 01:30:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 26 09:50:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

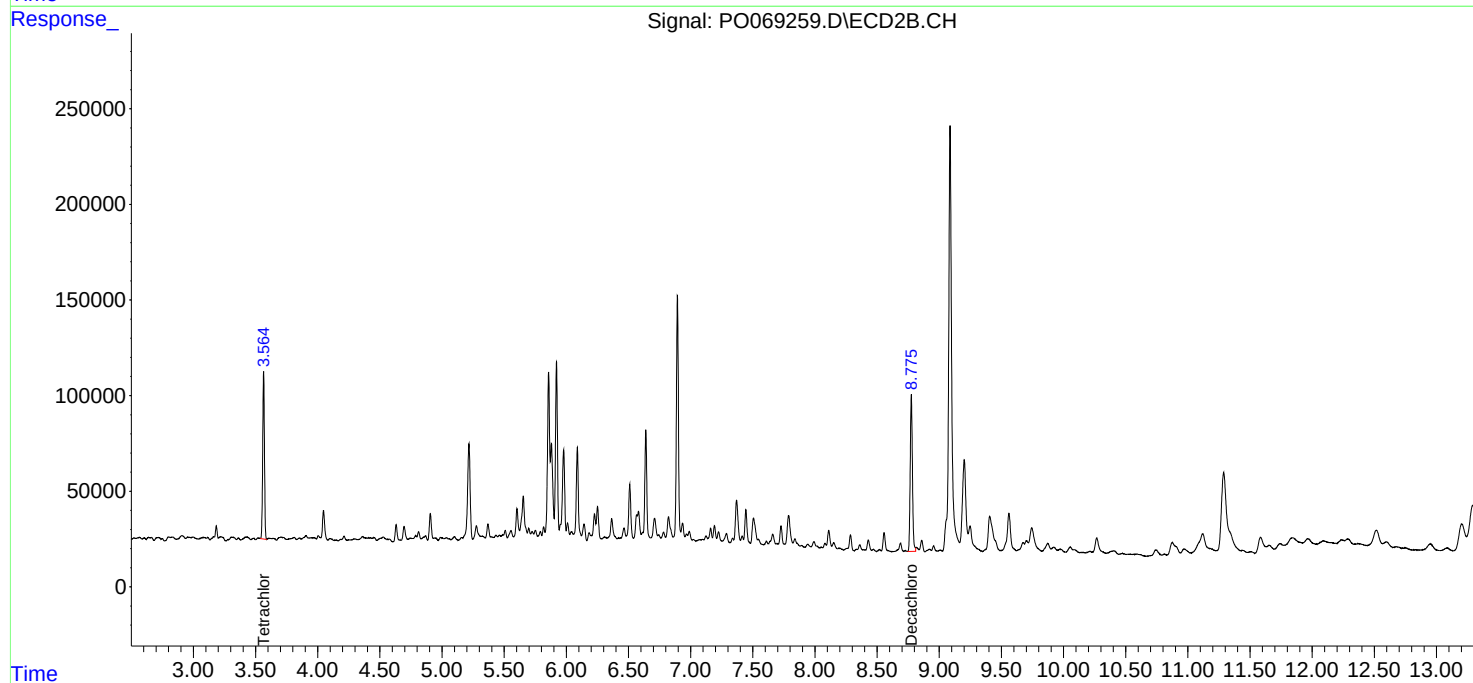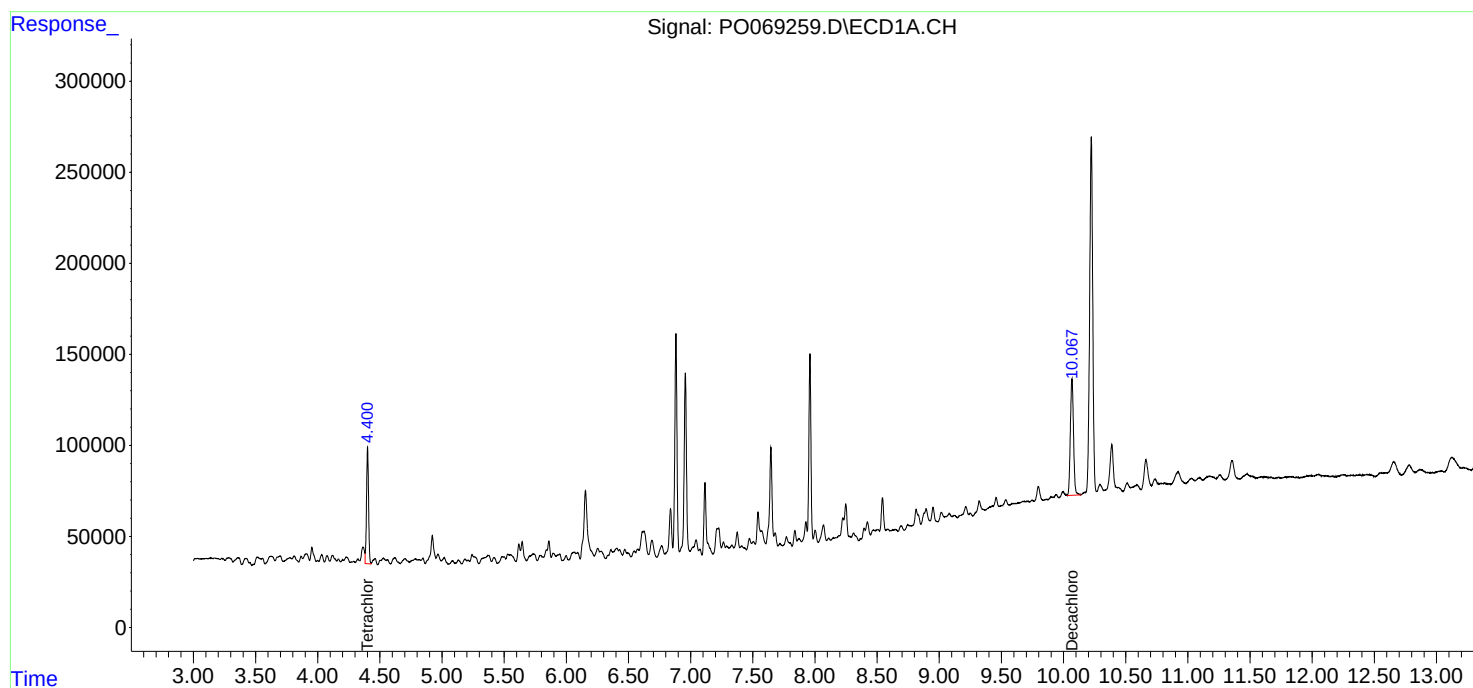

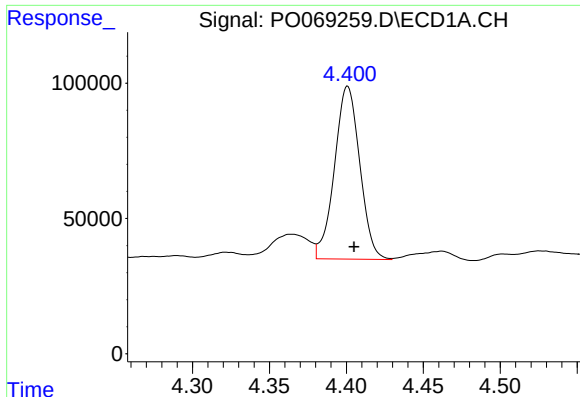


#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.004 min
Response: 729140
Conc: 24.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
WOOSPK-016-0004


Manual Integrations
APPROVED

Ankita
6/30/2020 1:45:08 PM

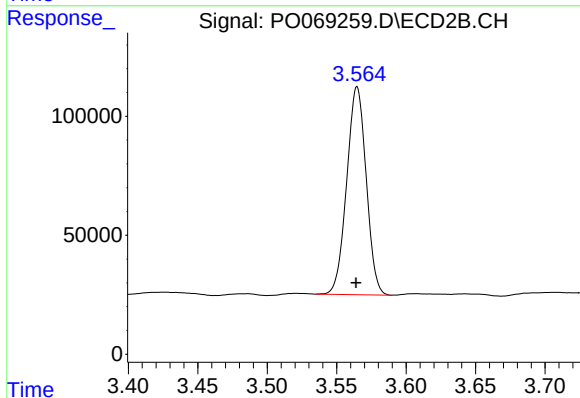


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 852800
Conc: 22.16 ng/ml

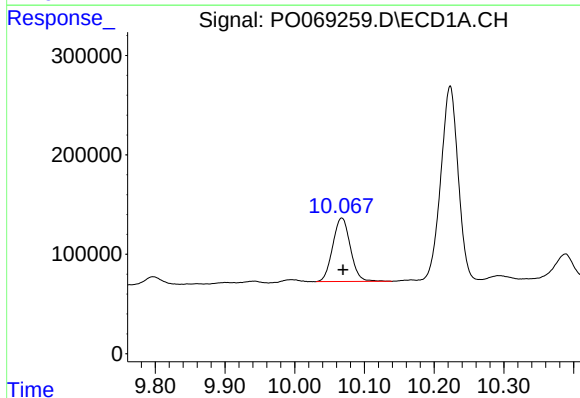

#2 Decachlorobiphenyl

R.T.: 10.068 min
Delta R.T.: -0.002 min
Response: 1126303
Conc: 23.71 ng/ml

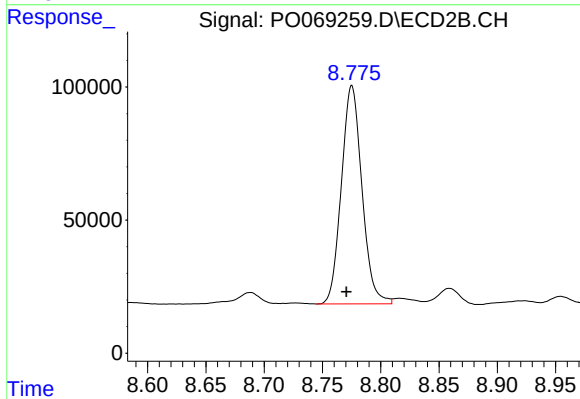

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: 0.004 min
Response: 1007295
Conc: 18.50 ng/ml m