

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062718\
Data File : P0046302.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2018 8:30
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

UGO
6/28/2018 3:58:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 09:29:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.380	3.603	13036379	5504419	22.304	22.177m
2) SA Decachlor...	10.048	8.572	9668112	3652157	20.969	21.787

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062718\
Data File : P0046302.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2018 8:30
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

UGO
6/28/2018 3:58:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 09:29:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

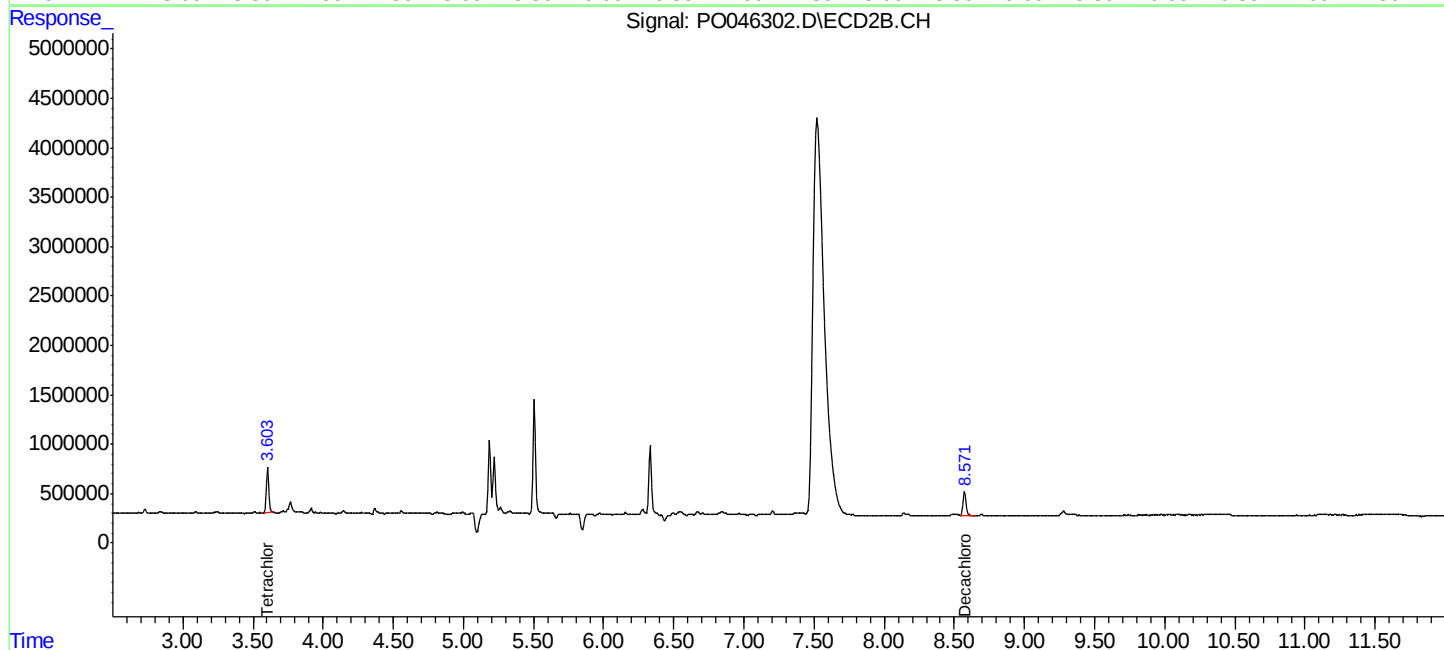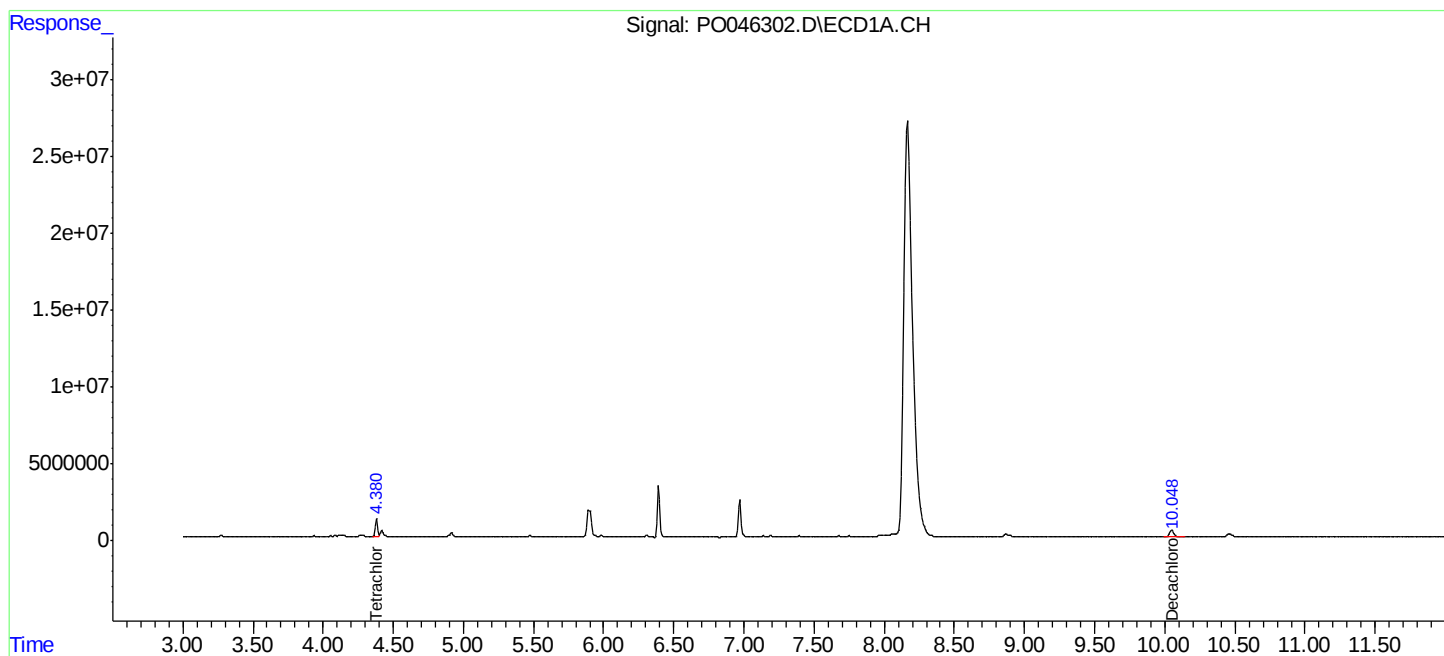

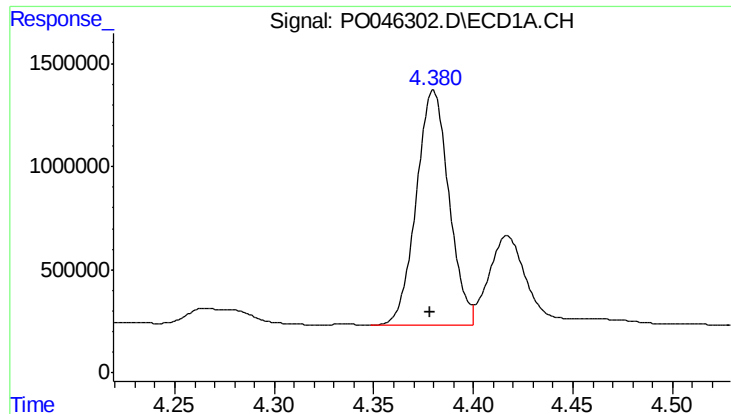


#1 Tetrachloro-m-xylene

R.T.: 4.380 min
Delta R.T.: 0.002 min
Response: 13036379
Conc: 22.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

UGO
6/28/2018 3:58:57 PM

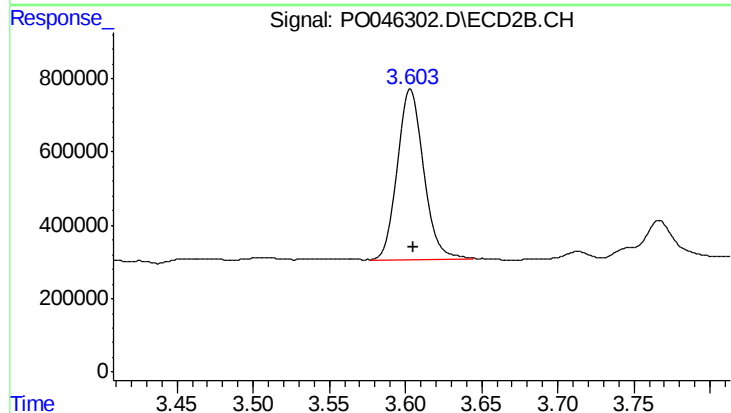


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.002 min
Response: 5504419
Conc: 22.18 ng/ml m

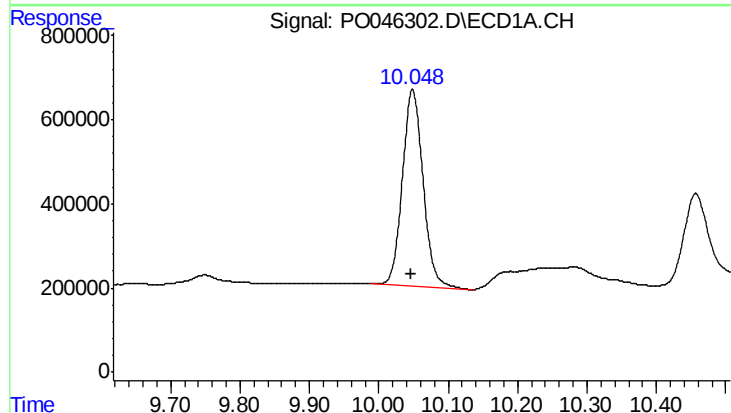

#2 Decachlorobiphenyl

R.T.: 10.048 min
Delta R.T.: 0.003 min
Response: 9668112
Conc: 20.97 ng/ml

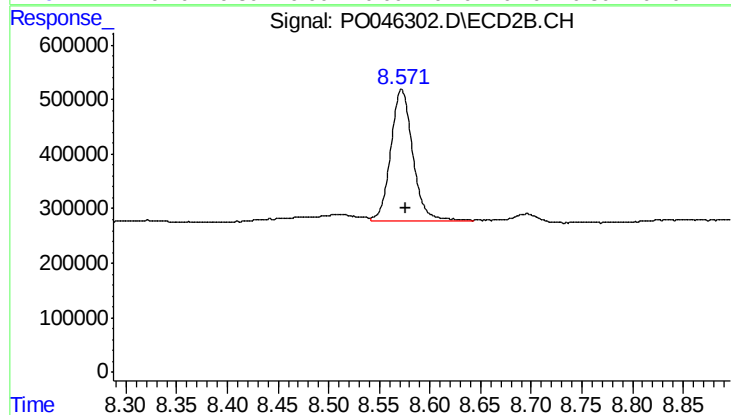

#2 Decachlorobiphenyl

R.T.: 8.572 min
Delta R.T.: -0.005 min
Response: 3652157
Conc: 21.79 ng/ml