

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062718\
Data File : P0046305.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2018 13:26
Operator : SM/UA
Sample : J3676-05RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RO-5-8RE

Manual Integrations
APPROVED

UGO
6/28/2018 3:59:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 14:38:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.383	3.610	3984156	2041952	6.817m	8.227m
2)	SA Decachlor...	10.047	8.572	2492294	1015852	5.406	6.060m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062718\
Data File : P0046305.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2018 13:26
Operator : SM/UA
Sample : J3676-05RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-5-8RE


Manual Integrations
APPROVED

UGO
6/28/2018 3:59:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 14:38:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

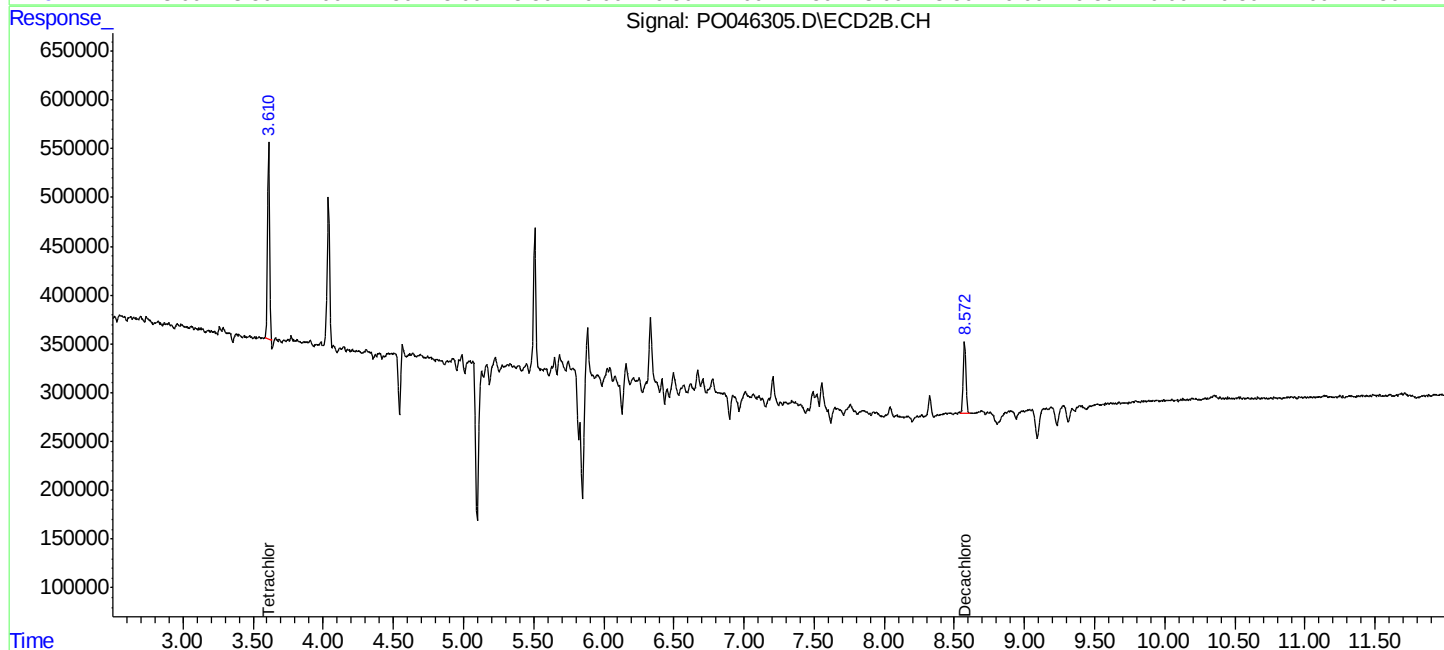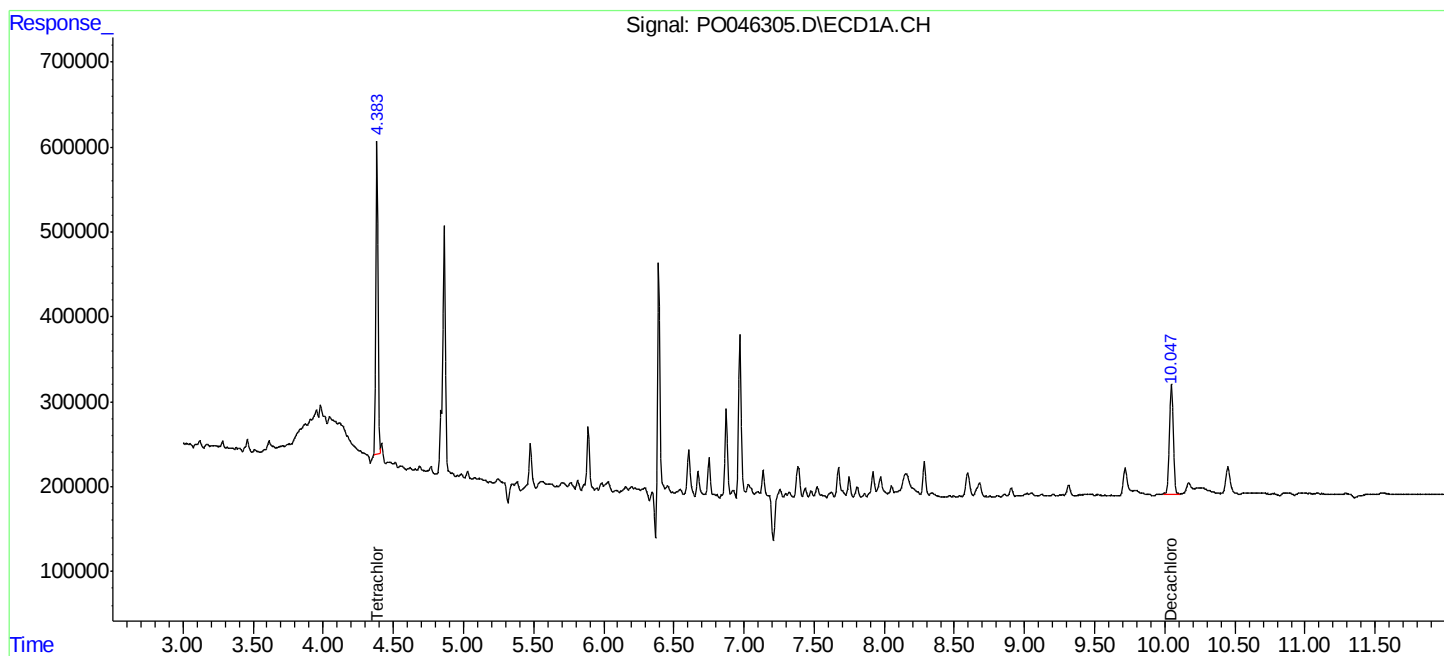

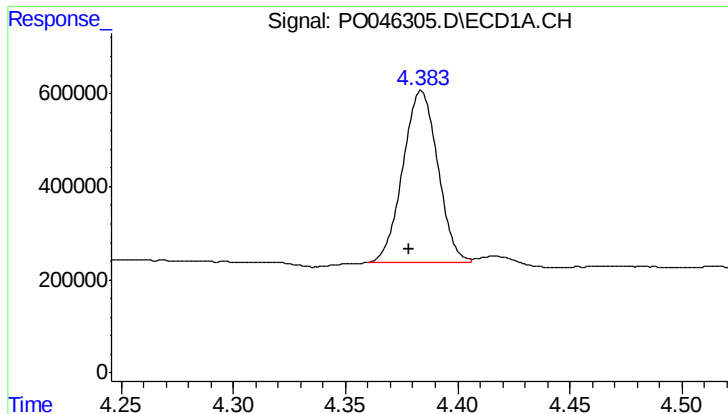


#1 Tetrachloro-m-xylene

R.T.: 4.383 min
Delta R.T.: 0.005 min
Response: 3984156
Conc: 6.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-5-8RE


Manual Integrations
APPROVED

UGO
6/28/2018 3:59:05 PM

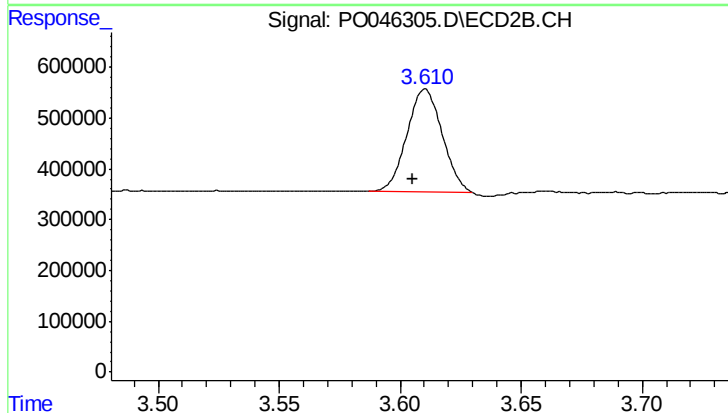


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: 0.005 min
Response: 2041952
Conc: 8.23 ng/ml m

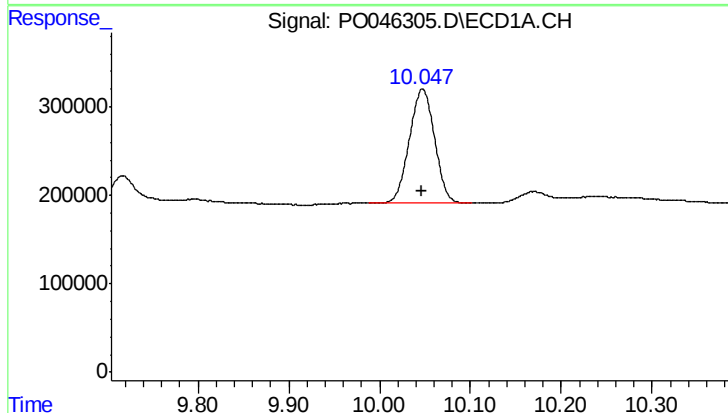

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: 0.001 min
Response: 2492294
Conc: 5.41 ng/ml

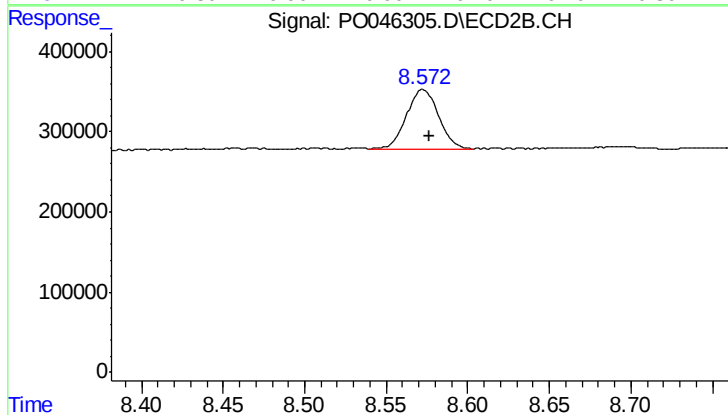

#2 Decachlorobiphenyl

R.T.: 8.572 min
Delta R.T.: -0.005 min
Response: 1015852
Conc: 6.06 ng/ml m