

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062818\
Data File : P0046355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2018 16:23
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 07:05:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062818.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 28 11:20:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.387	3.612	8985067	4055584	21.852	24.057
2) SA Decachlor...	10.052	8.574	6025836	2453762	22.962	23.130

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062818\
Data File : P0046355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2018 16:23
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 07:05:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062818.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 28 11:20:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

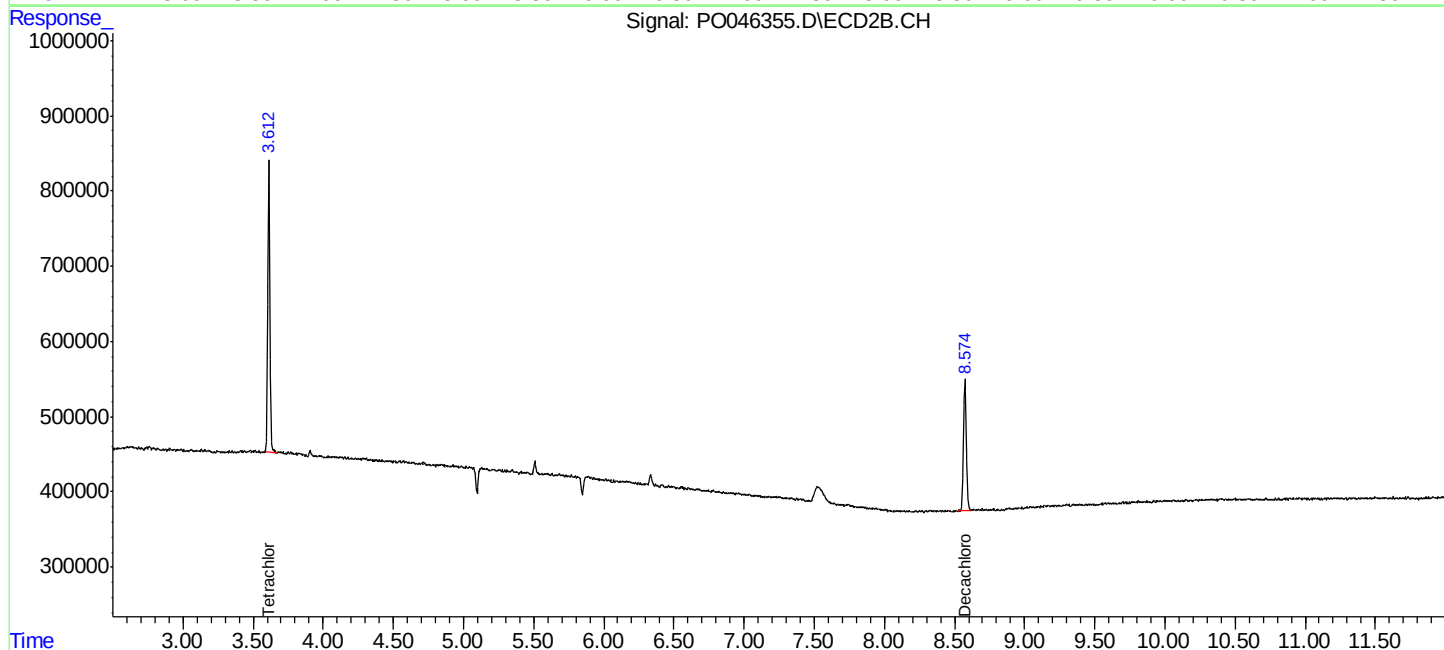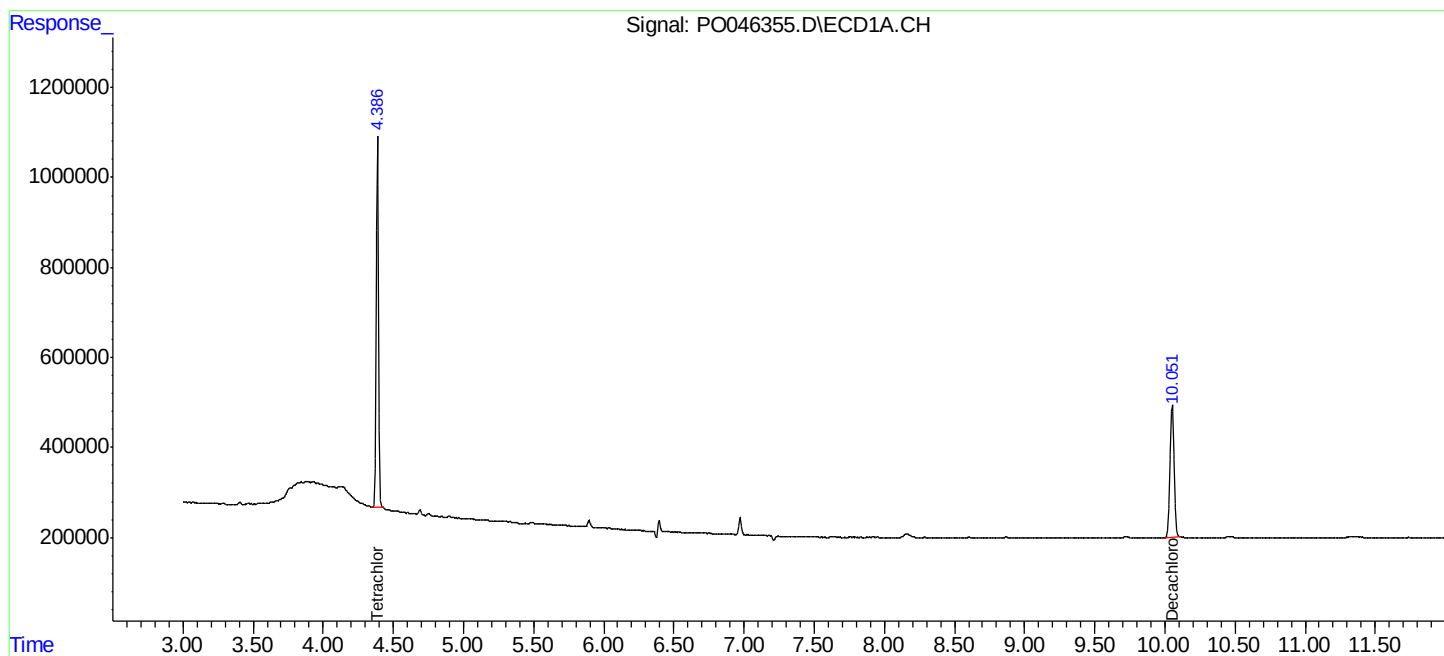


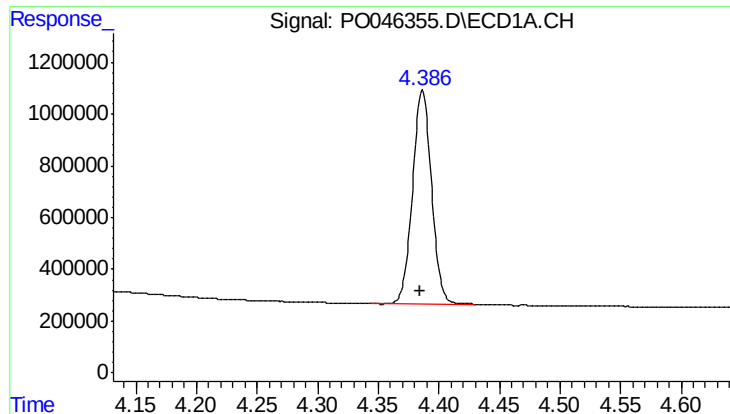

#1 Tetrachloro-m-xylene


R.T.: 4.387 min
Delta R.T.: 0.003 min
Response: 8985067
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

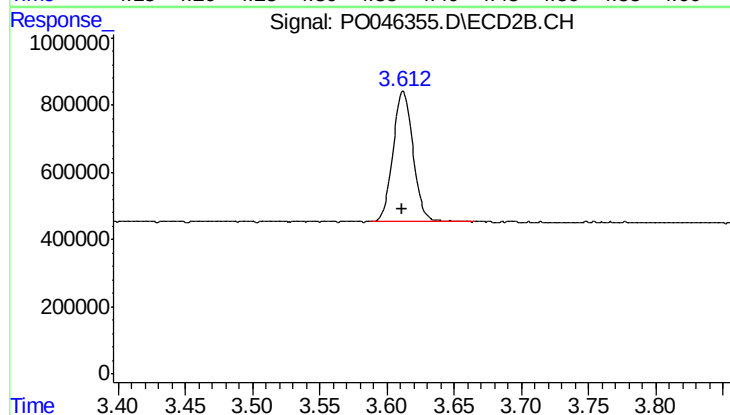


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: 0.001 min
Response: 4055584
Conc: 24.06 ng/ml

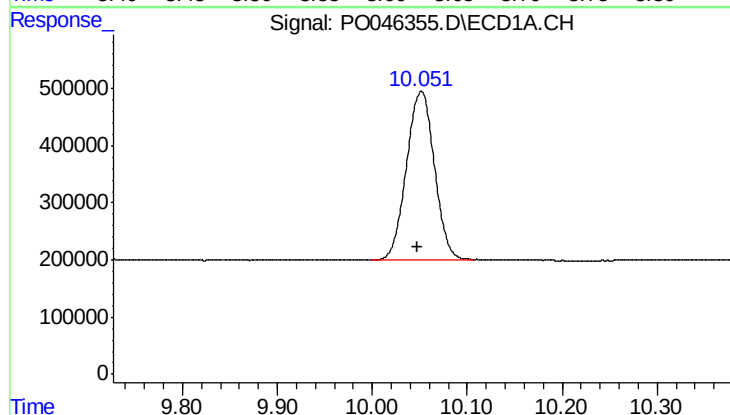

#2 Decachlorobiphenyl

R.T.: 10.052 min
Delta R.T.: 0.004 min
Response: 6025836
Conc: 22.96 ng/ml

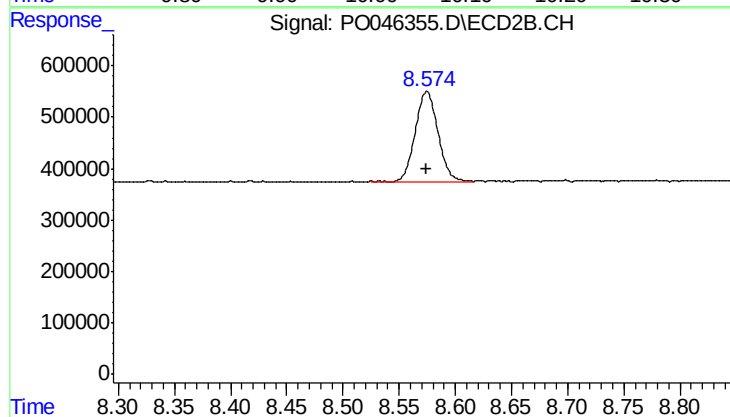

#2 Decachlorobiphenyl

R.T.: 8.574 min
Delta R.T.: 0.000 min
Response: 2453762
Conc: 23.13 ng/ml