

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062819\
 Data File : P0057586.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2019 13:36
 Operator : SM/SJ
 Sample : K3157-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-062619-A

Manual Integrations
 APPROVED

Ankita
 7/1/2019 11:47:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 02:10:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.229	3.550	1086614	870616	27.662m	24.760
2) SA Decachlor...	9.771	8.467	958628	609386	17.047	16.291

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062819\
Data File : P0057586.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2019 13:36
Operator : SM/SJ
Sample : K3157-11
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-062619-A


Manual Integrations
APPROVED

Ankita
7/1/2019 11:47:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 02:10:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

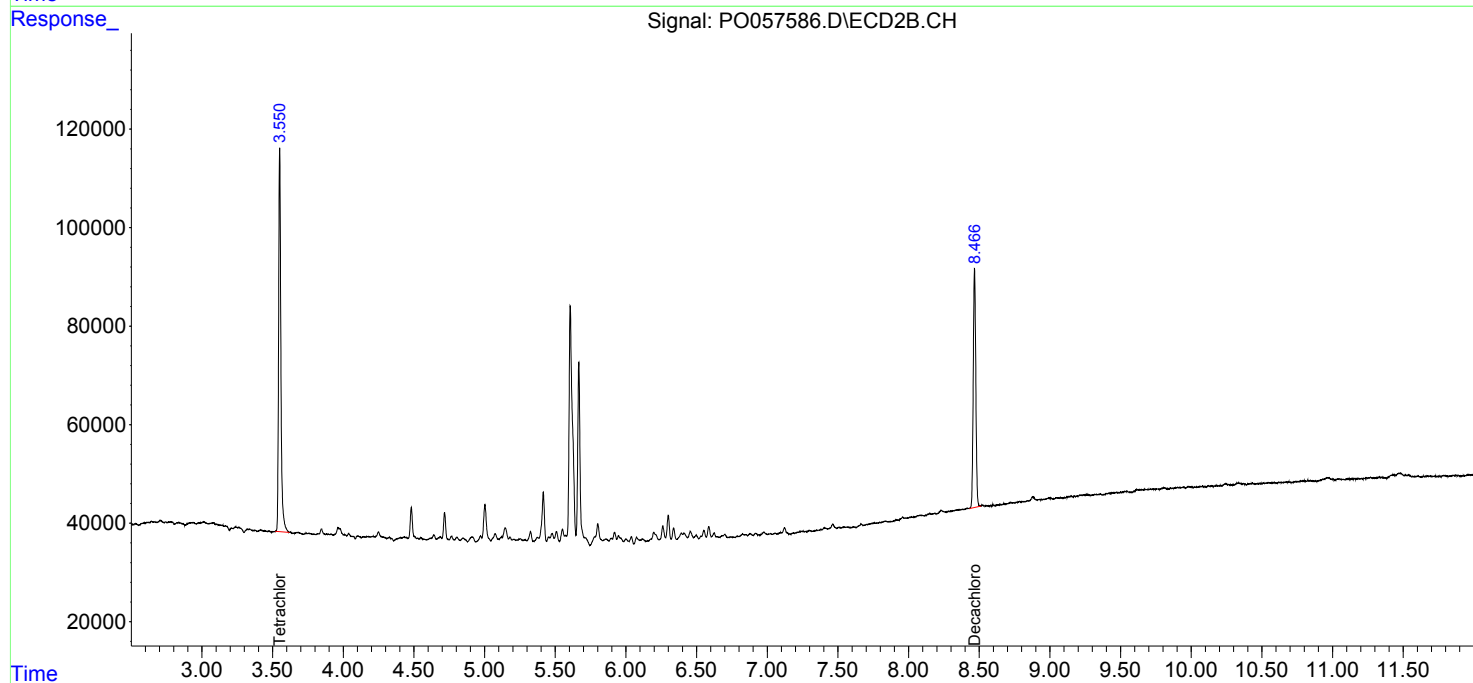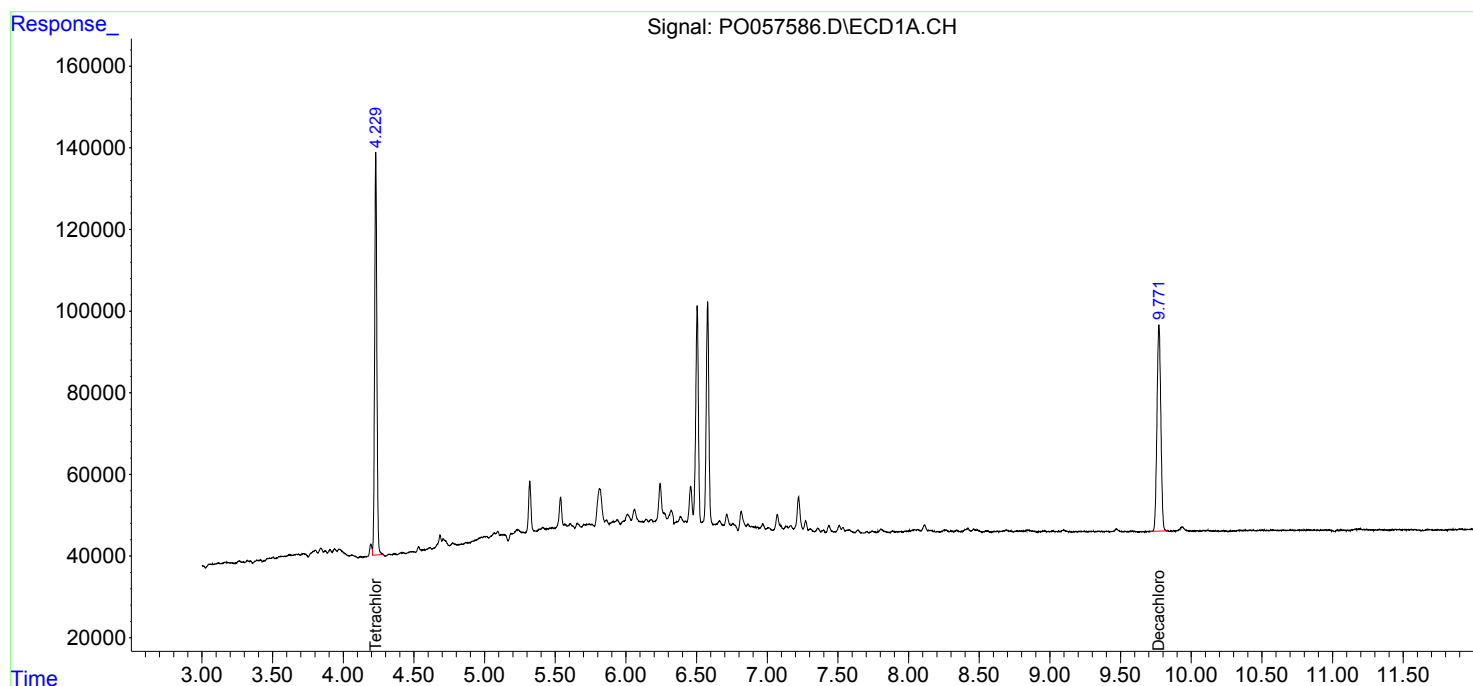

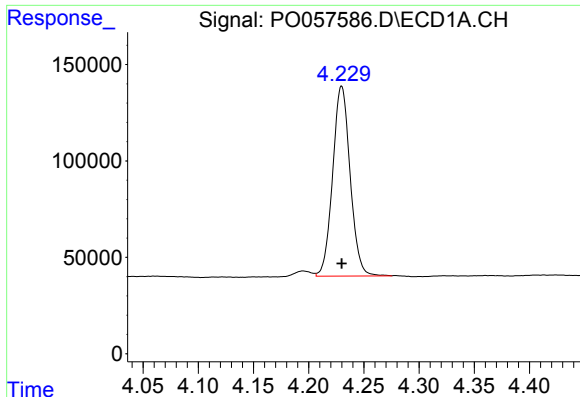


#1 Tetrachloro-m-xylene

R.T.: 4.229 min
Delta R.T.: 0.000 min
Response: 1086614
Conc: 27.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-02-062619-A


Manual Integrations
APPROVED

Ankita
7/1/2019 11:47:02 AM

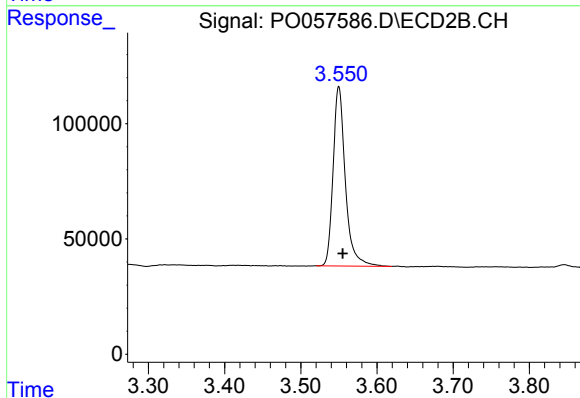


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: -0.005 min
Response: 870616
Conc: 24.76 ng/ml

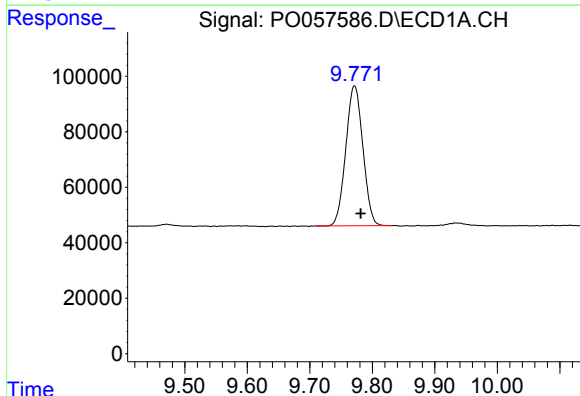

#2 Decachlorobiphenyl

R.T.: 9.771 min
Delta R.T.: -0.010 min
Response: 958628
Conc: 17.05 ng/ml

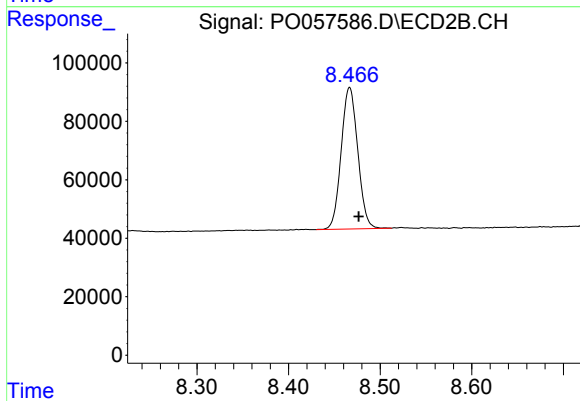

#2 Decachlorobiphenyl

R.T.: 8.467 min
Delta R.T.: -0.010 min
Response: 609386
Conc: 16.29 ng/ml