

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062819\
 Data File : P0057587.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2019 13:53
 Operator : SM/SJ
 Sample : K3157-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-062619-B

Manual Integrations
 APPROVED

Ankita
 7/1/2019 11:47:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 03:18:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.219	3.549	1210068	970215	30.805m	27.592
2) SA Decachlor...	9.757	8.463	1128179	699835	20.063	18.709

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062819\
Data File : PO057587.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2019 13:53
Operator : SM/SJ
Sample : K3157-13
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-062619-B


Manual Integrations
APPROVED

Ankita
7/1/2019 11:47:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 03:18:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

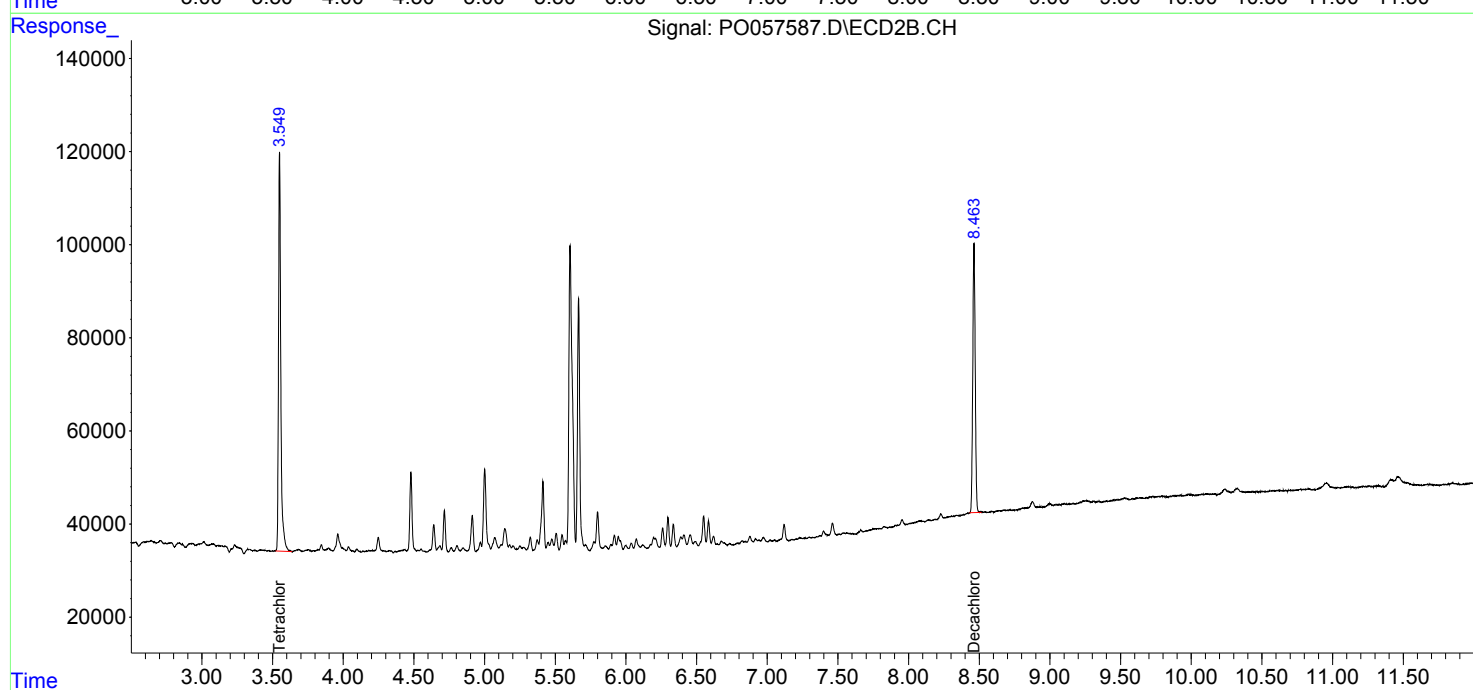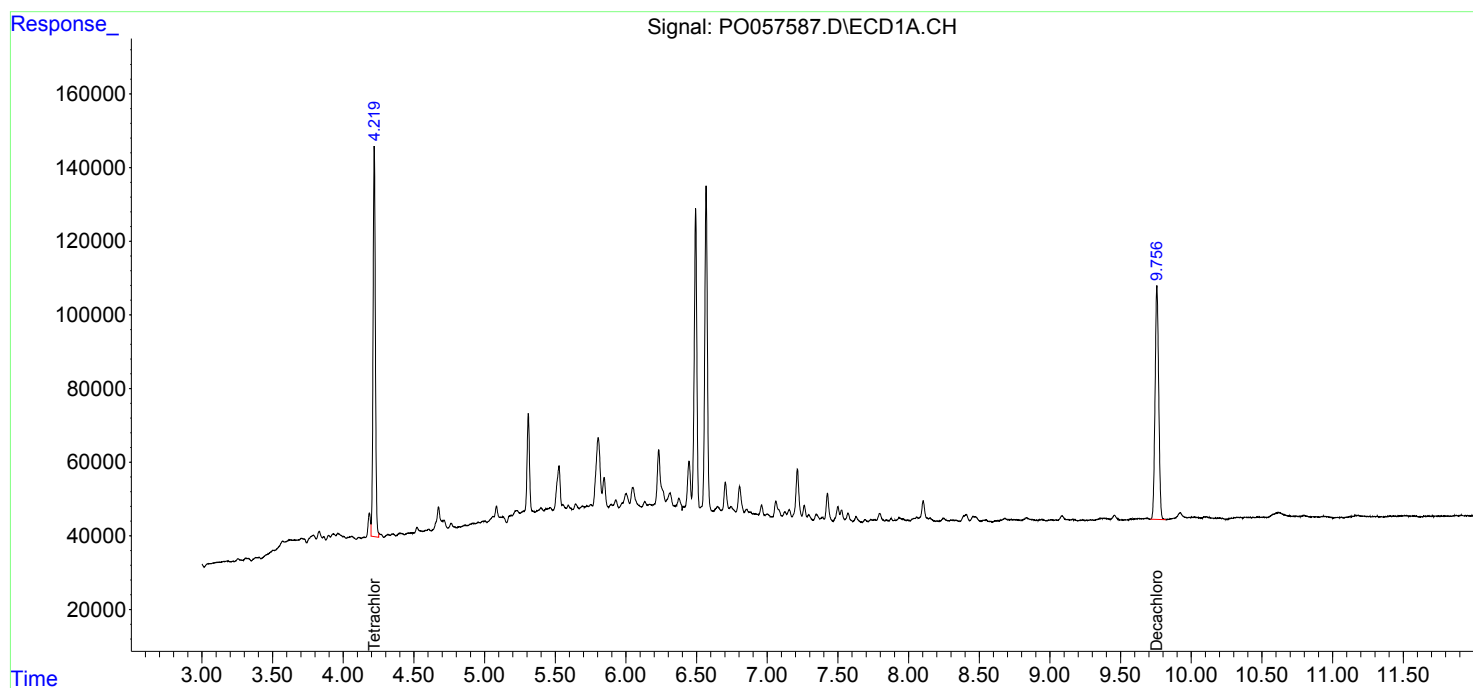

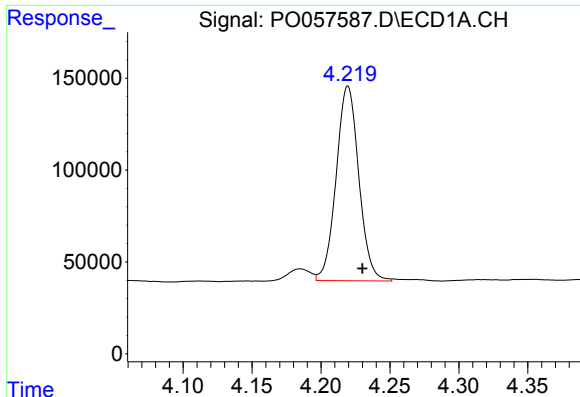


#1 Tetrachloro-m-xylene

R.T.: 4.219 min
Delta R.T.: -0.011 min
Response: 1210068
Conc: 30.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-02-062619-B


Manual Integrations
APPROVED

Ankita
7/1/2019 11:47:33 AM

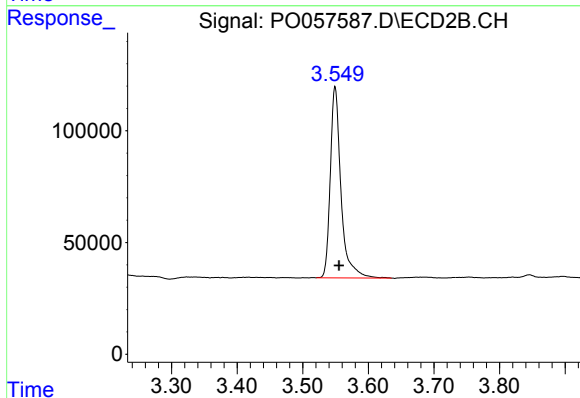


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.006 min
Response: 970215
Conc: 27.59 ng/ml

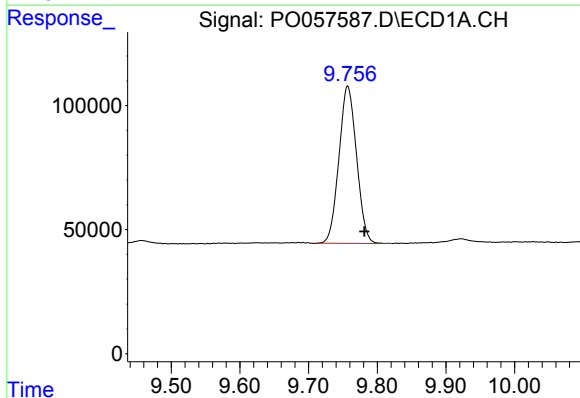

#2 Decachlorobiphenyl

R.T.: 9.757 min
Delta R.T.: -0.024 min
Response: 1128179
Conc: 20.06 ng/ml

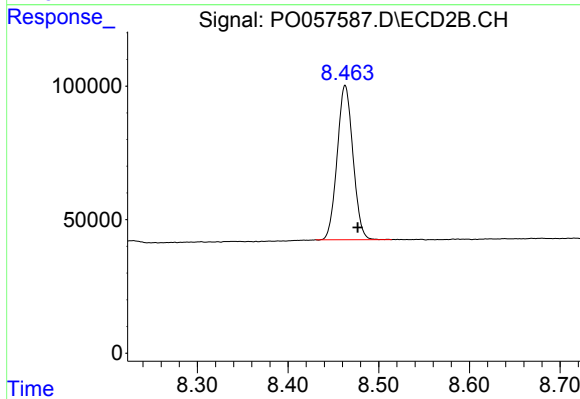

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: -0.014 min
Response: 699835
Conc: 18.71 ng/ml