

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062819\
 Data File : P0057619.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2019 23:19
 Operator : SM/SJ
 Sample : K3583-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-A-01-B-01-C

Manual Integrations
 APPROVED

Ankita
 7/1/2019 11:48:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 04:54:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.216	3.548	693476	606868	17.654m	17.259
2) SA Decachlor...	9.752	8.462	1218364	681183	21.666	18.210

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062819\
Data File : P0057619.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2019 23:19
Operator : SM/SJ
Sample : K3583-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
7/1/2019 11:48:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 04:54:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

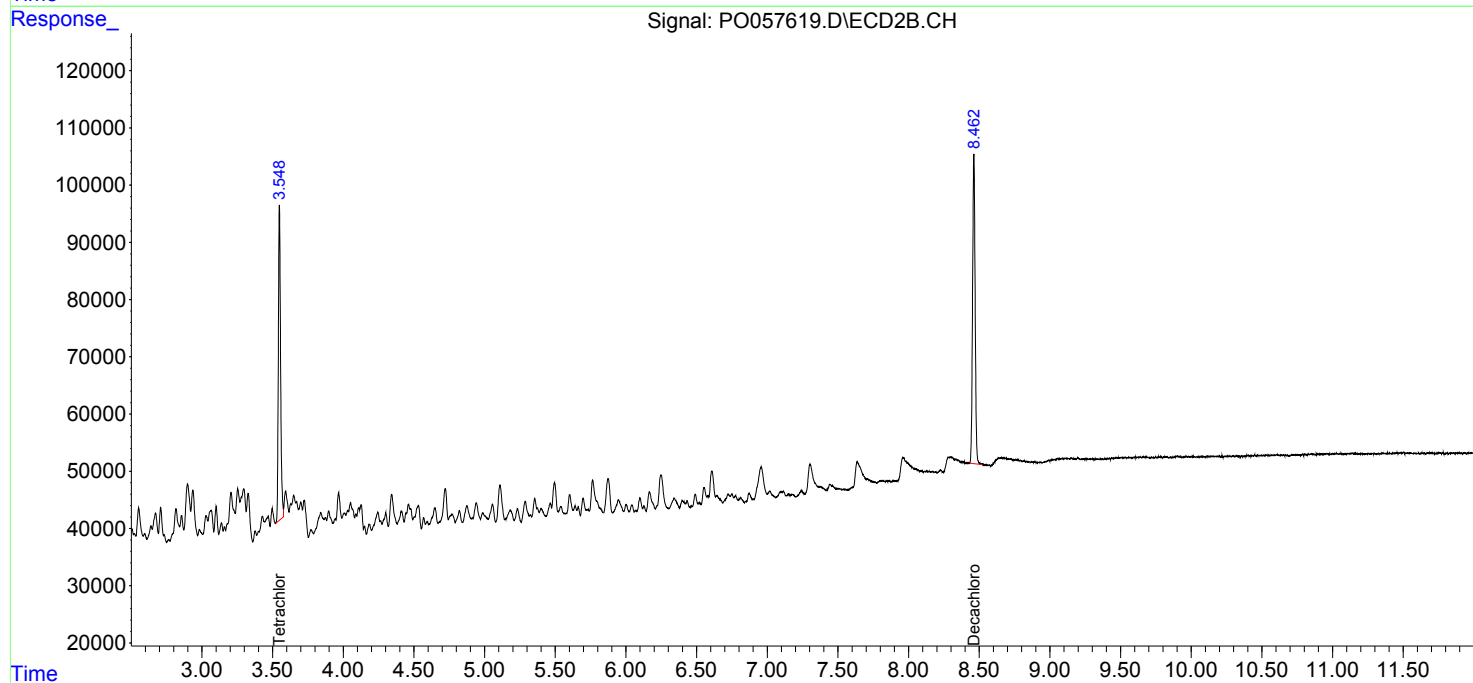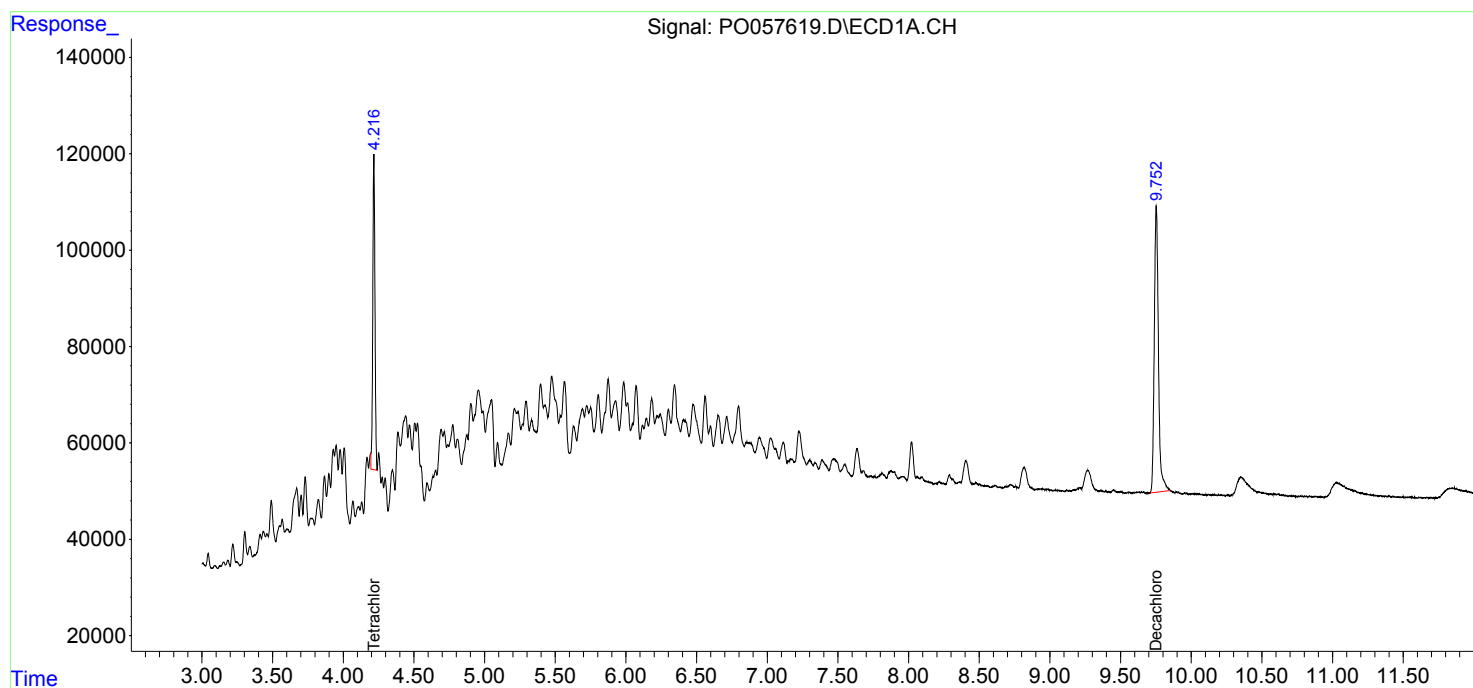

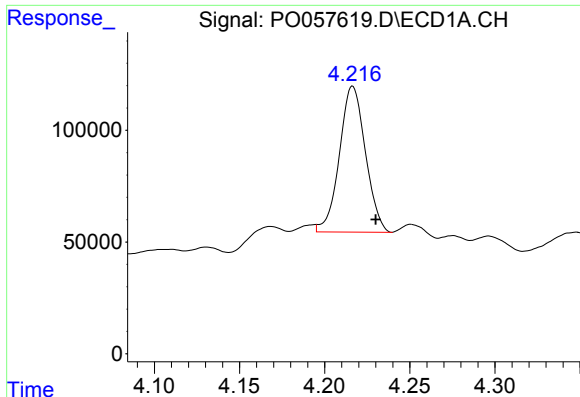


#1 Tetrachloro-m-xylene

R.T.: 4.216 min
Delta R.T.: -0.014 min
Response: 693476
Conc: 17.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
7/1/2019 11:48:07 AM

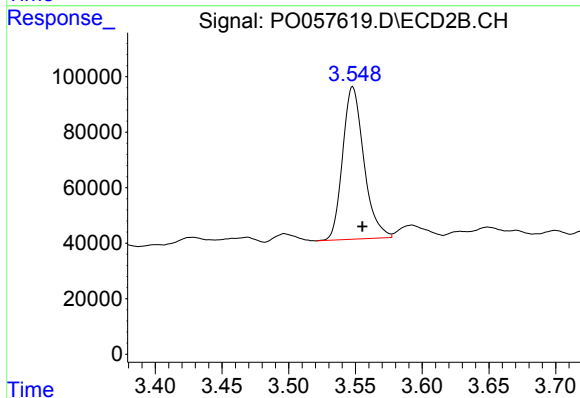


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.007 min
Response: 606868
Conc: 17.26 ng/ml

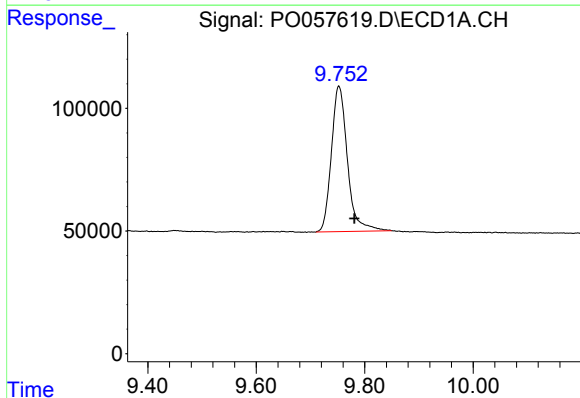

#2 Decachlorobiphenyl

R.T.: 9.752 min
Delta R.T.: -0.029 min
Response: 1218364
Conc: 21.67 ng/ml

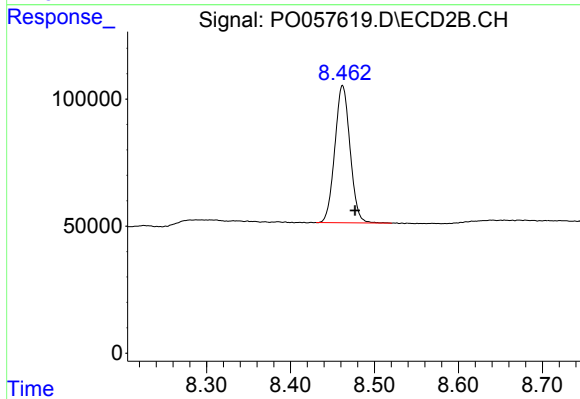

#2 Decachlorobiphenyl

R.T.: 8.462 min
Delta R.T.: -0.015 min
Response: 681183
Conc: 18.21 ng/ml