

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
 Data File : P0057702.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jul 2019 14:06
 Operator : SM/SJ
 Sample : K3633-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 02-A-02-B-02-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 14:34:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.213	3.546	961046	698055	24.466m	19.852
2) SA Decachlor...	9.751	8.461	1327730	897960	23.611	24.005

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
Data File : P0057702.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jul 2019 14:06
Operator : SM/SJ
Sample : K3633-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 14:34:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

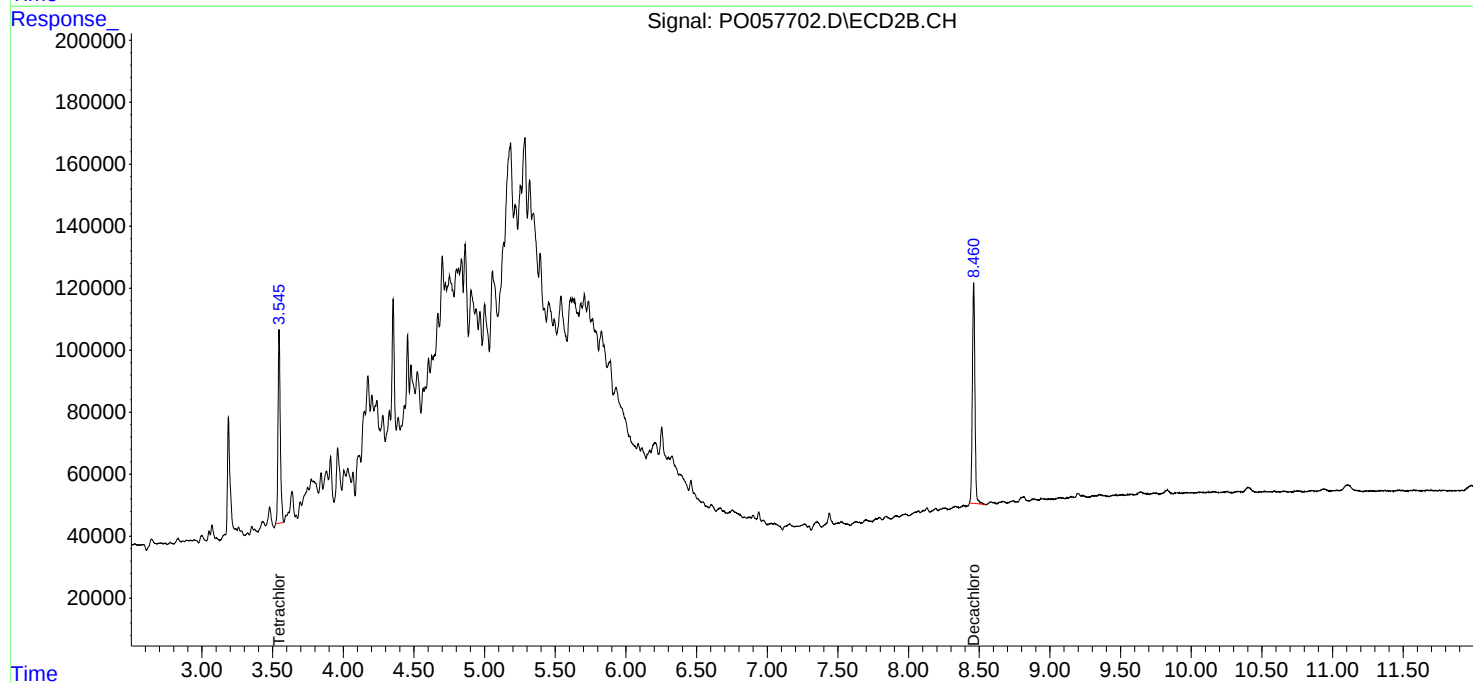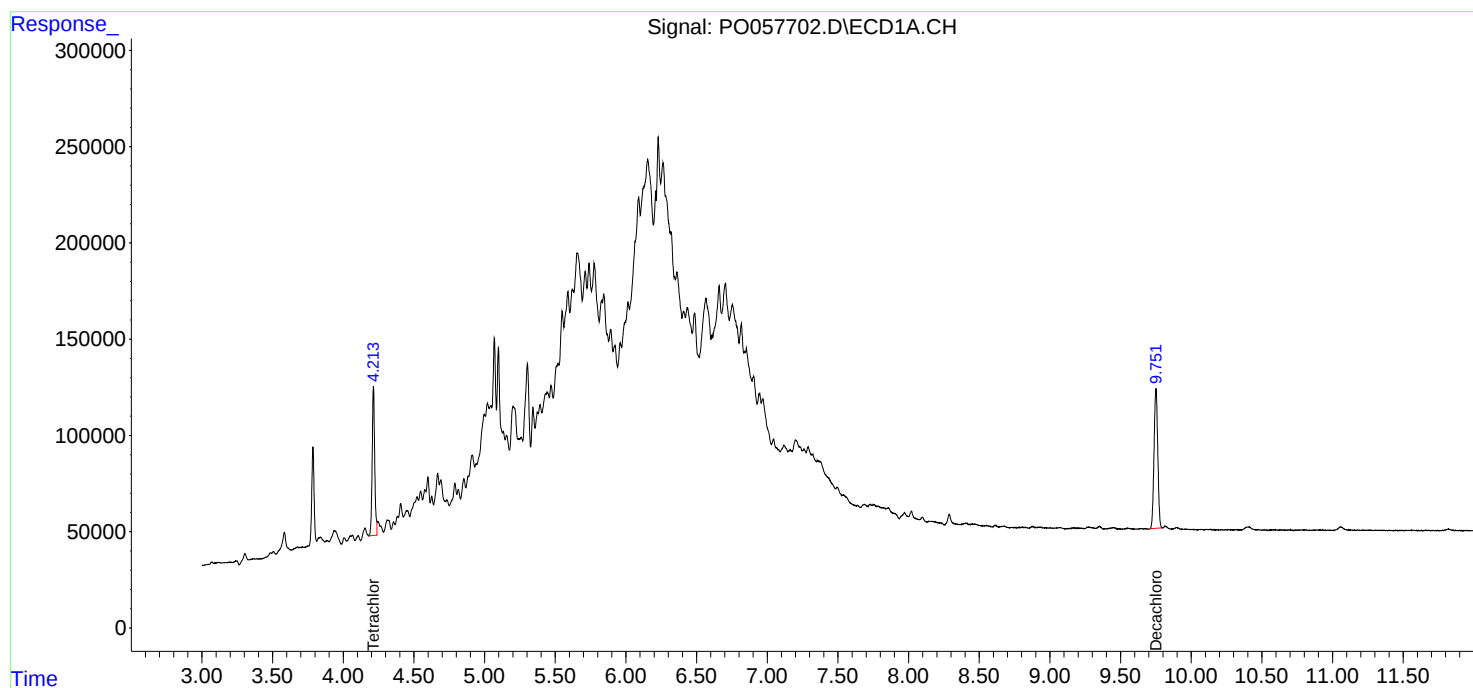


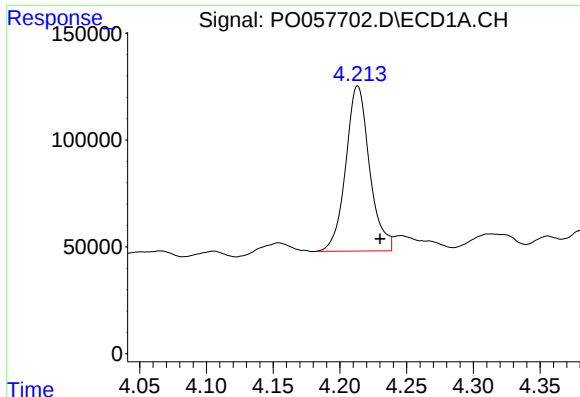

#1 Tetrachloro-m-xylene


R.T.: 4.213 min
Delta R.T.: -0.017 min
Response: 961046
Conc: 24.47 ng/ml m

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C

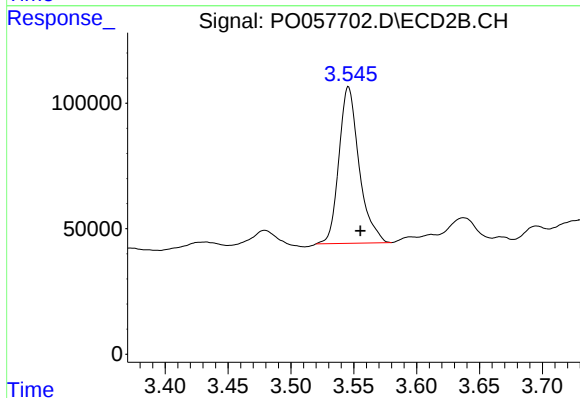


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.009 min
Response: 698055
Conc: 19.85 ng/ml

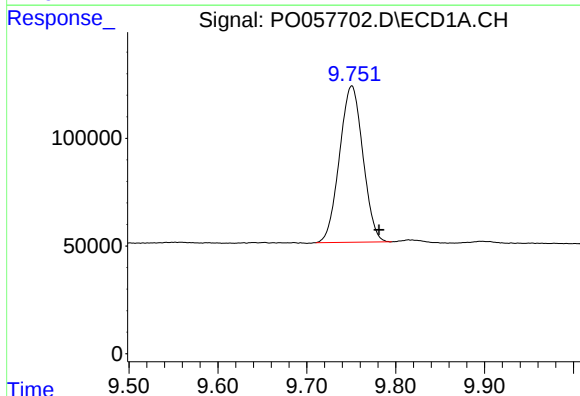

#2 Decachlorobiphenyl

R.T.: 9.751 min
Delta R.T.: -0.031 min
Response: 1327730
Conc: 23.61 ng/ml

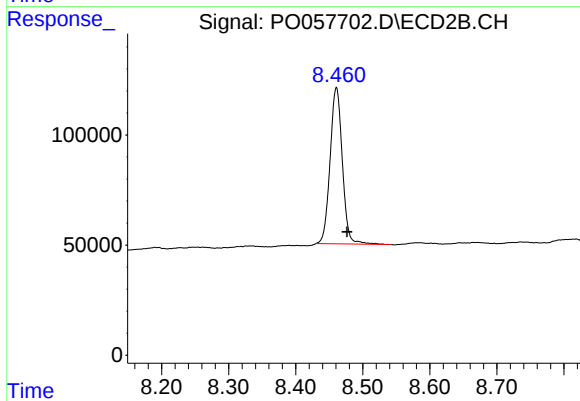

#2 Decachlorobiphenyl

R.T.: 8.461 min
Delta R.T.: -0.016 min
Response: 897960
Conc: 24.01 ng/ml