

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
 Data File : P0057705.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jul 2019 14:57
 Operator : SM/SJ
 Sample : K3633-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 05-A-05-B-05-C

Manual Integrations
 APPROVED

Ankita
 7/8/2019 11:08:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 15:12:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.214	3.549	1096289	841941	27.908m	23.944
2) SA Decachlor...	9.749	8.464	1081424	682842	19.231m	18.254

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070319\
Data File : PO057705.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jul 2019 14:57
Operator : SM/SJ
Sample : K3633-05
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
05-A-05-B-05-C


Manual Integrations
APPROVED

Ankita
7/8/2019 11:08:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 15:12:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

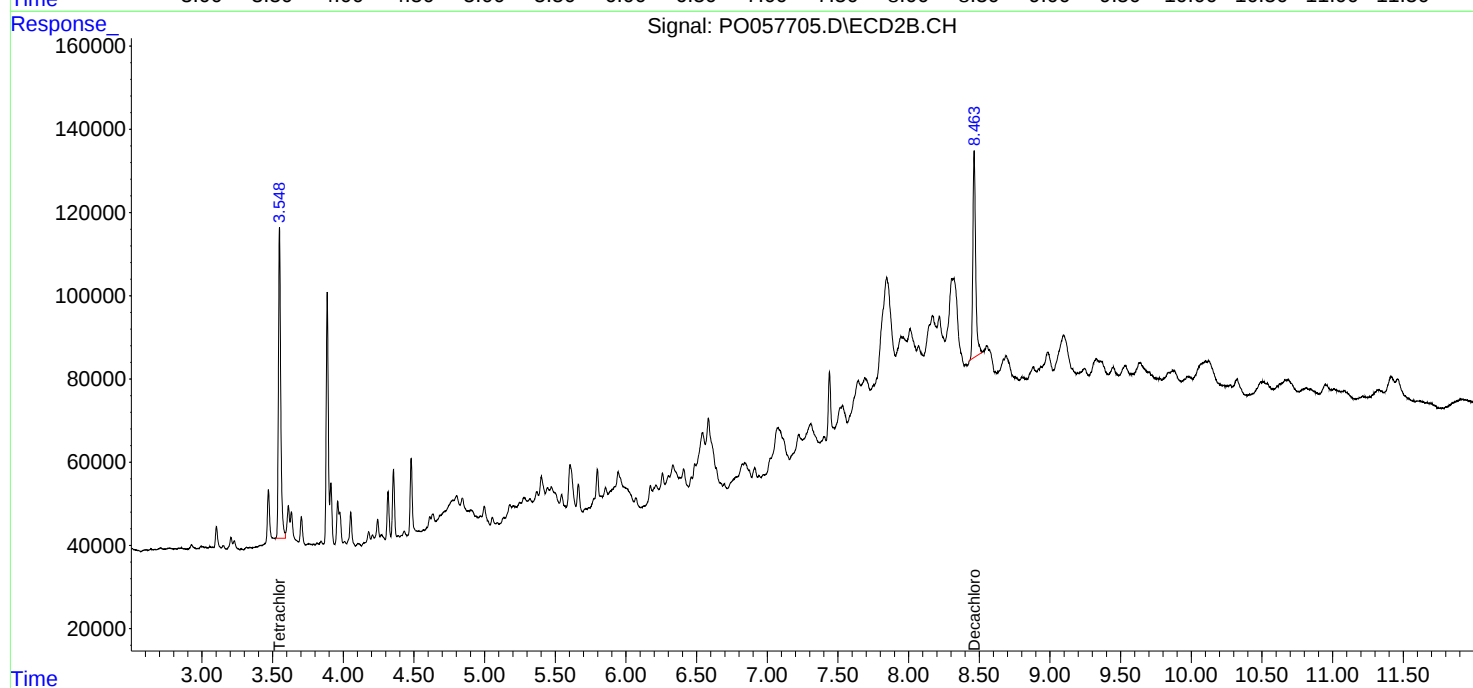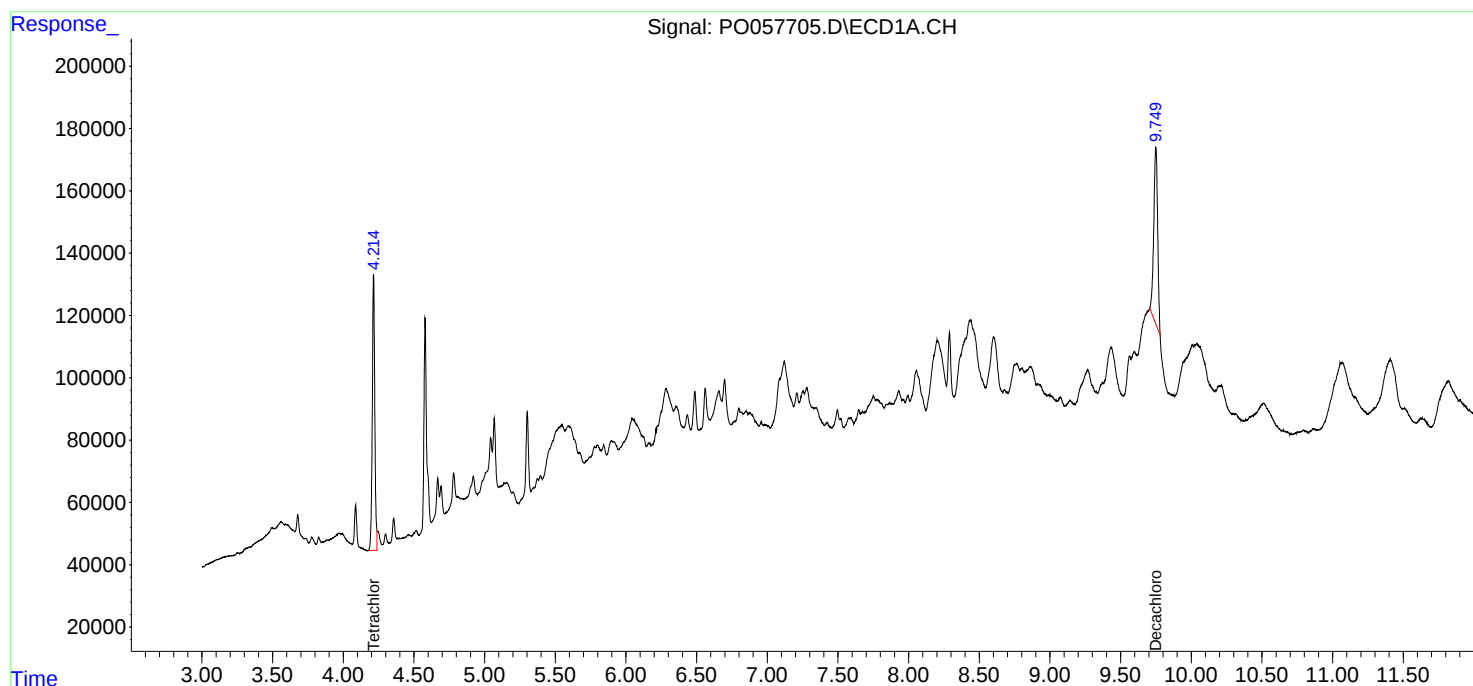

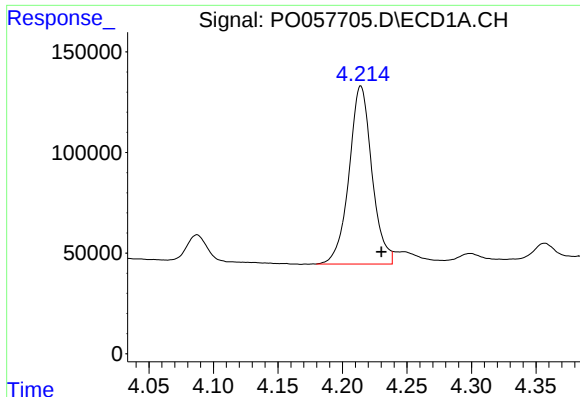

#1 Tetrachloro-m-xylene

R.T.: 4.214 min

Delta R.T.: -0.016 min


Response: 1096289

Conc: 27.91 ng/ml m

Instrument :
ECD_O
ClientSampleId :
05-A-05-B-05-C

Manual Integrations
APPROVED

Ankita
7/8/2019 11:08:52 AM

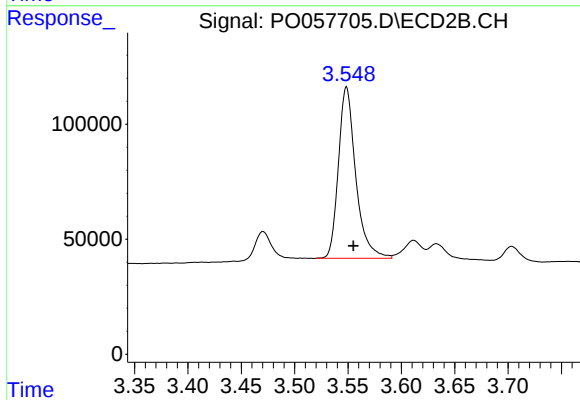


#1 Tetrachloro-m-xylene

R.T.: 3.549 min

Delta R.T.: -0.007 min

Response: 841941

Conc: 23.94 ng/ml

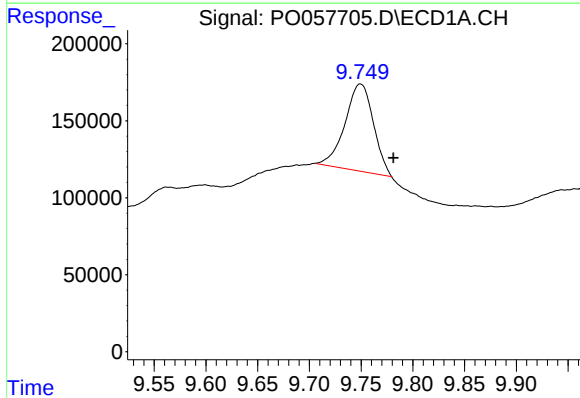


#2 Decachlorobiphenyl

R.T.: 9.749 min

Delta R.T.: -0.033 min

Response: 1081424

Conc: 19.23 ng/ml m

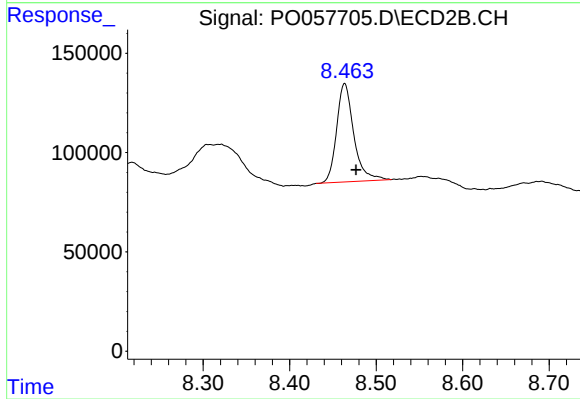

#2 Decachlorobiphenyl

R.T.: 8.464 min

Delta R.T.: -0.013 min

Response: 682842

Conc: 18.25 ng/ml