

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
 Data File : P0057706.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jul 2019 15:14
 Operator : SM/SJ
 Sample : K3633-04RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 04-A-04-B-04-CRE

Manual Integrations
 APPROVED

Ankita
 7/8/2019 11:08:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 15:33:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.216	3.550	672885	590979	17.130	16.807
2) SA Decachlor...	9.766	8.475	163561	108414	2.909m	2.898m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
Data File : P0057706.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jul 2019 15:14
Operator : SM/SJ
Sample : K3633-04RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
04-A-04-B-04-CRE


Manual Integrations
APPROVED

Ankita
7/8/2019 11:08:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 15:33:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

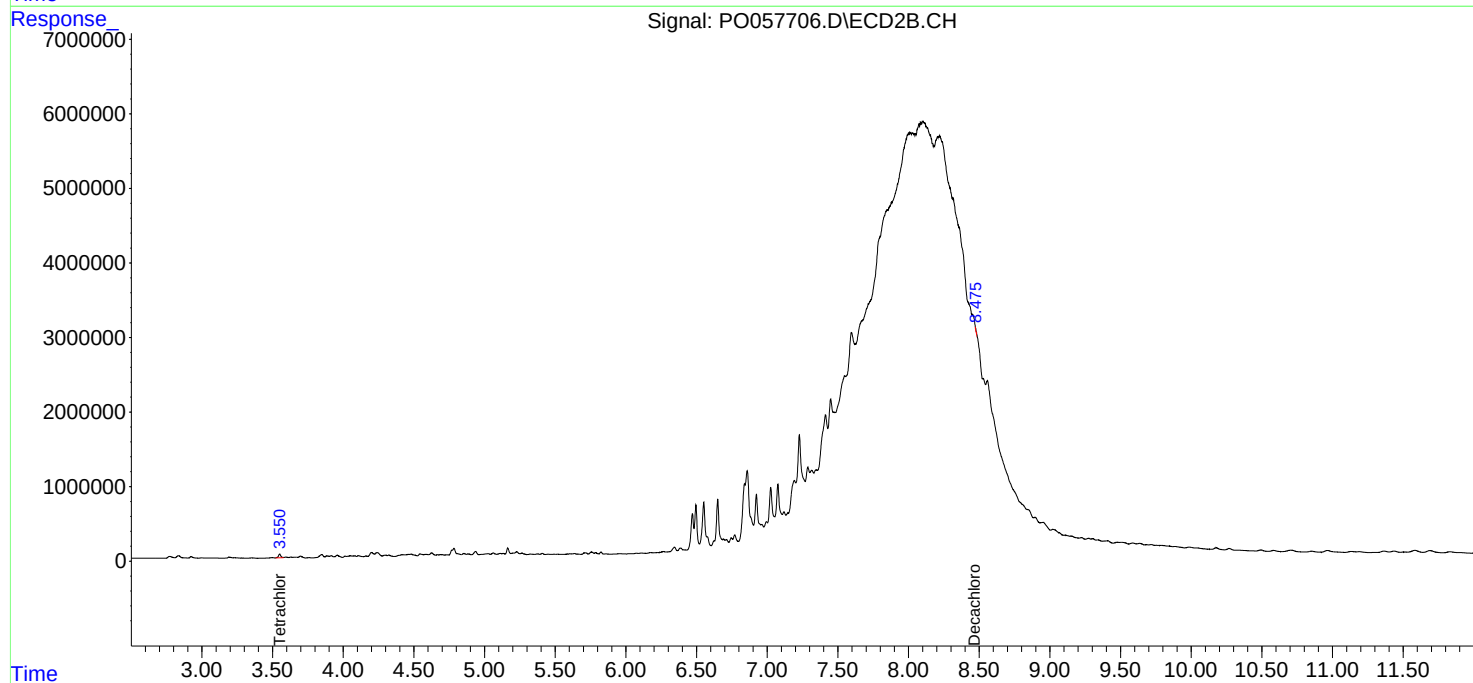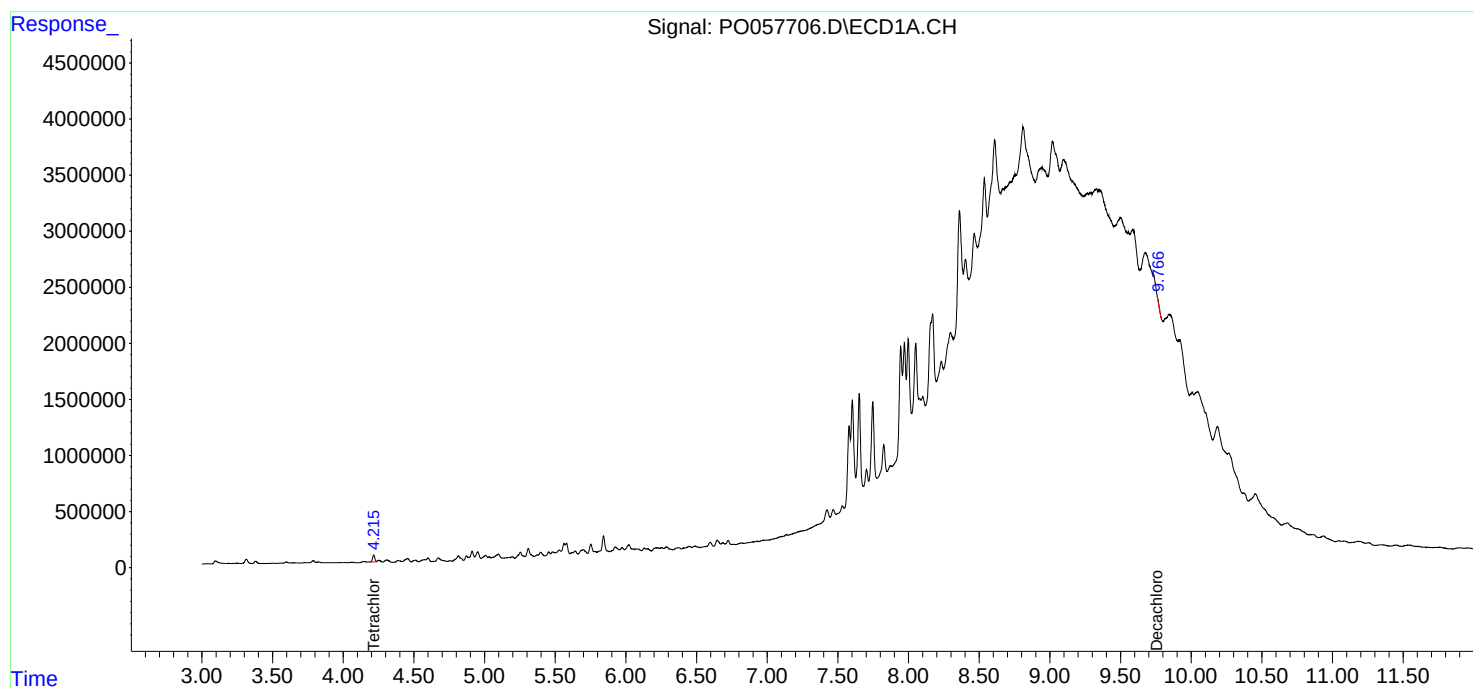

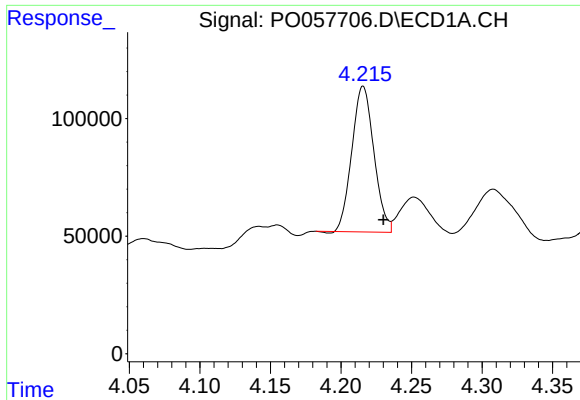


#1 Tetrachloro-m-xylene

R.T.: 4.216 min
Delta R.T.: -0.014 min
Response: 672885
Conc: 17.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
04-A-04-B-04-CRE


Manual Integrations
APPROVED

Ankita
7/8/2019 11:08:54 AM

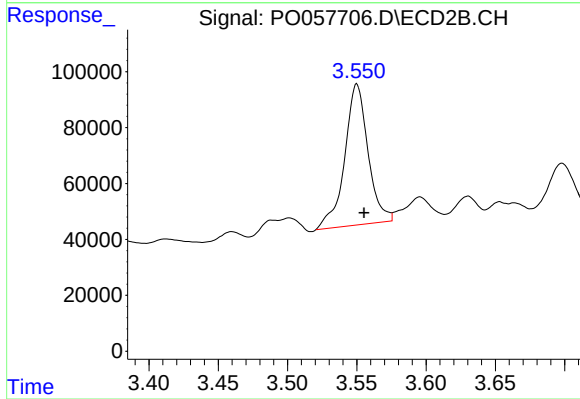


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: -0.005 min
Response: 590979
Conc: 16.81 ng/ml

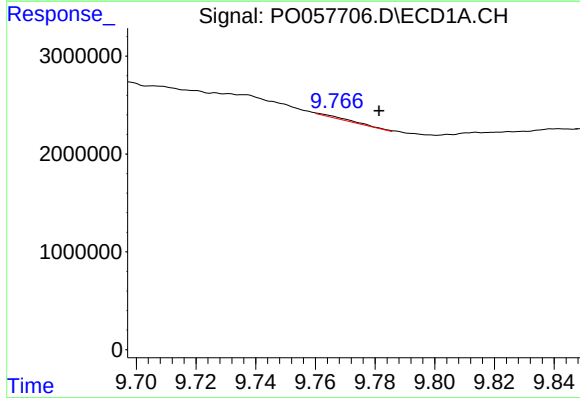

#2 Decachlorobiphenyl

R.T.: 9.766 min
Delta R.T.: -0.015 min
Response: 163561
Conc: 2.91 ng/ml m

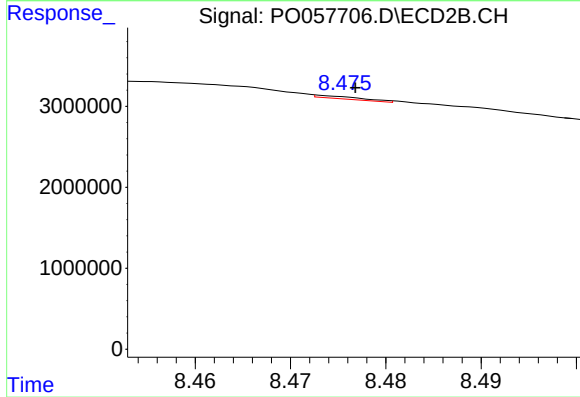

#2 Decachlorobiphenyl

R.T.: 8.475 min
Delta R.T.: -0.001 min
Response: 108414
Conc: 2.90 ng/ml m