

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
 Data File : P0057707.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jul 2019 16:37
 Operator : SM/SJ
 Sample : K3649-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 D-1-ROLL-OFF-SOCK-PILE

Manual Integrations
 APPROVED

Ankita
 7/8/2019 11:08:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 16:55:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.218	3.549	746542	611321	19.005	17.385
2) SA Decachlor...	9.754	8.463	945648	384137	16.817m	10.269m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
Data File : P0057707.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jul 2019 16:37
Operator : SM/SJ
Sample : K3649-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
D-1-ROLL-OFF-SOCK-PILE


Manual Integrations
APPROVED

Ankita
7/8/2019 11:08:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 16:55:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

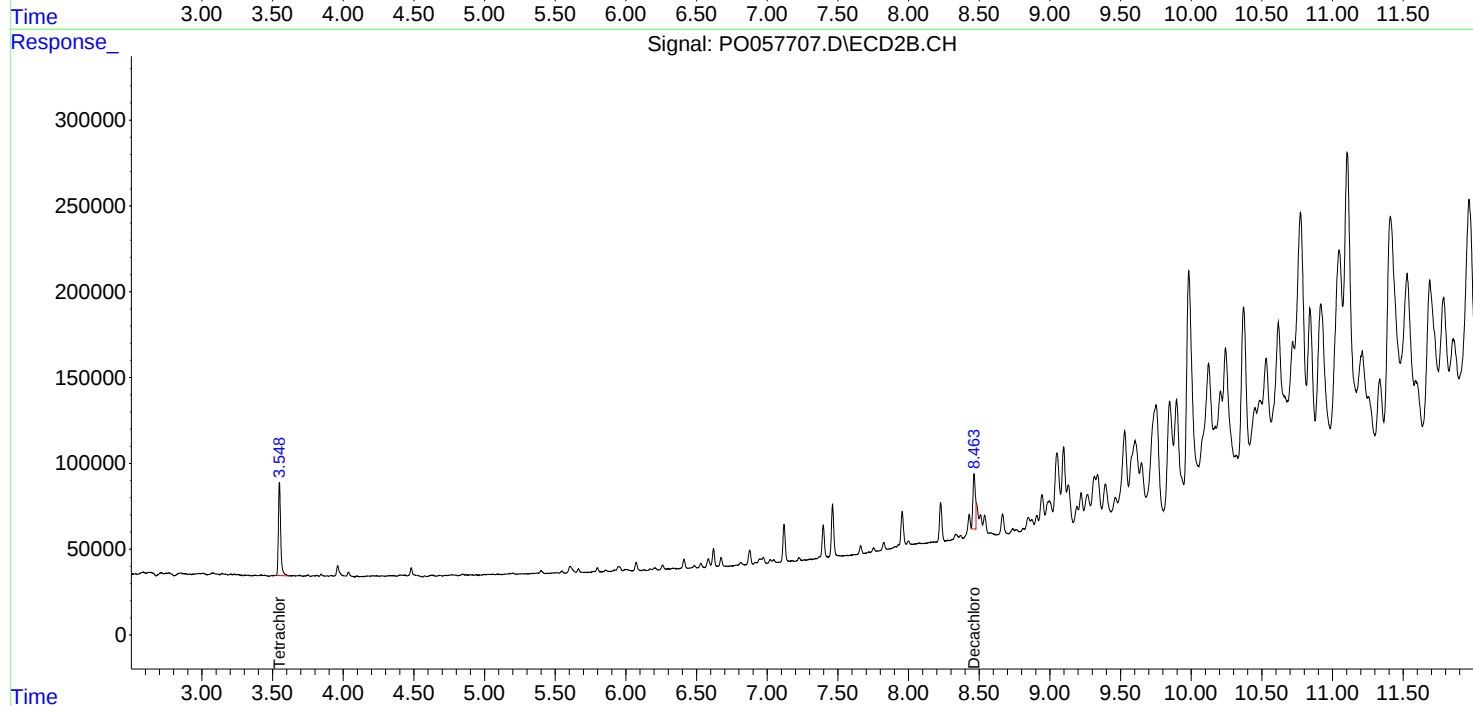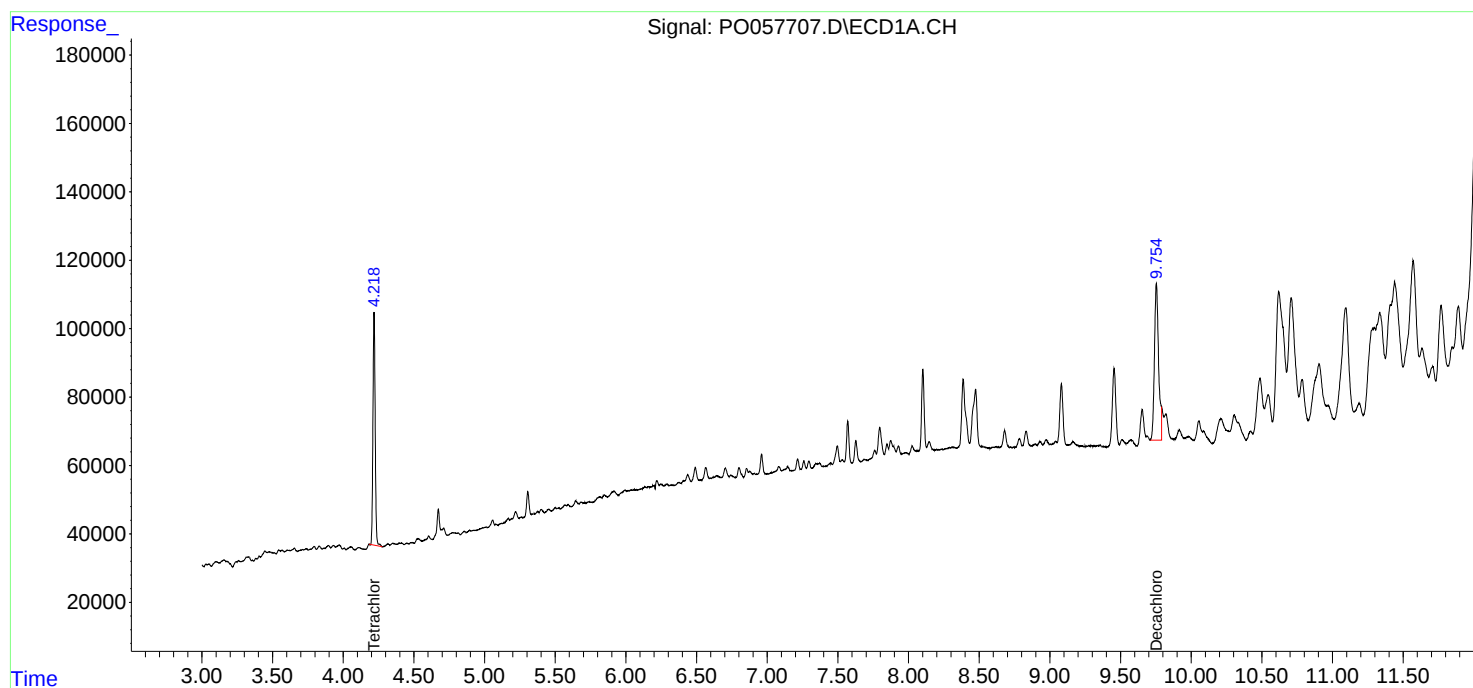

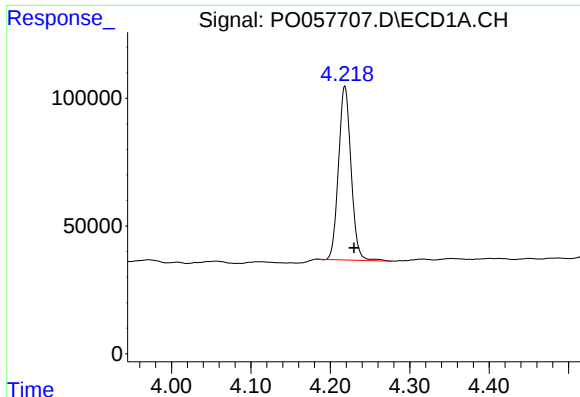


#1 Tetrachloro-m-xylene

R.T.: 4.218 min
Delta R.T.: -0.012 min
Response: 746542
Conc: 19.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
D-1-ROLL-OFF-SOCK-PILE


Manual Integrations
APPROVED

Ankita
7/8/2019 11:08:57 AM

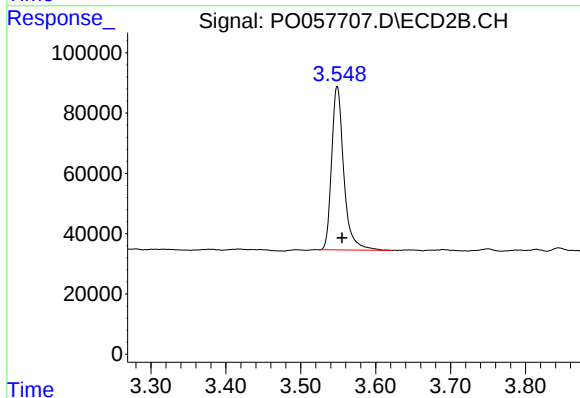


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.007 min
Response: 611321
Conc: 17.39 ng/ml

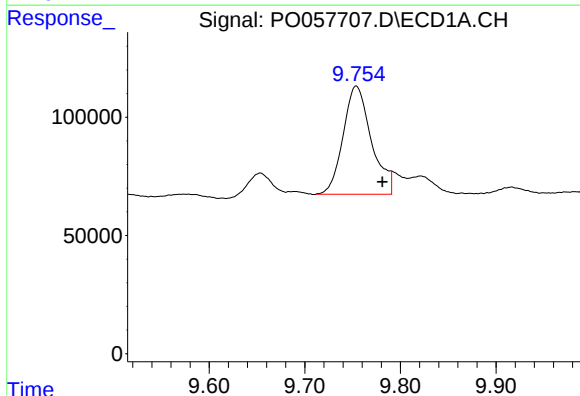

#2 Decachlorobiphenyl

R.T.: 9.754 min
Delta R.T.: -0.028 min
Response: 945648
Conc: 16.82 ng/ml m

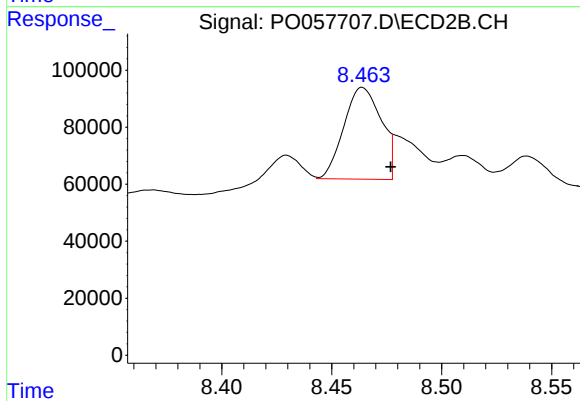

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: -0.013 min
Response: 384137
Conc: 10.27 ng/ml m