

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070319\
 Data File : P0057717.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jul 2019 20:25
 Operator : SM/SJ
 Sample : K3653-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HL4-1(3-3.5)

Manual Integrations
 APPROVED

Ankita
 7/8/2019 11:09:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:35:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.214	3.548	871350	736213	22.182	20.937
2) SA Decachlor...	9.748	8.460	672977	465255	11.968	12.438m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070319\
Data File : PO057717.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jul 2019 20:25
Operator : SM/SJ
Sample : K3653-06
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HL4-1(3-3.5)


Manual Integrations
APPROVED

Ankita
7/8/2019 11:09:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:35:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

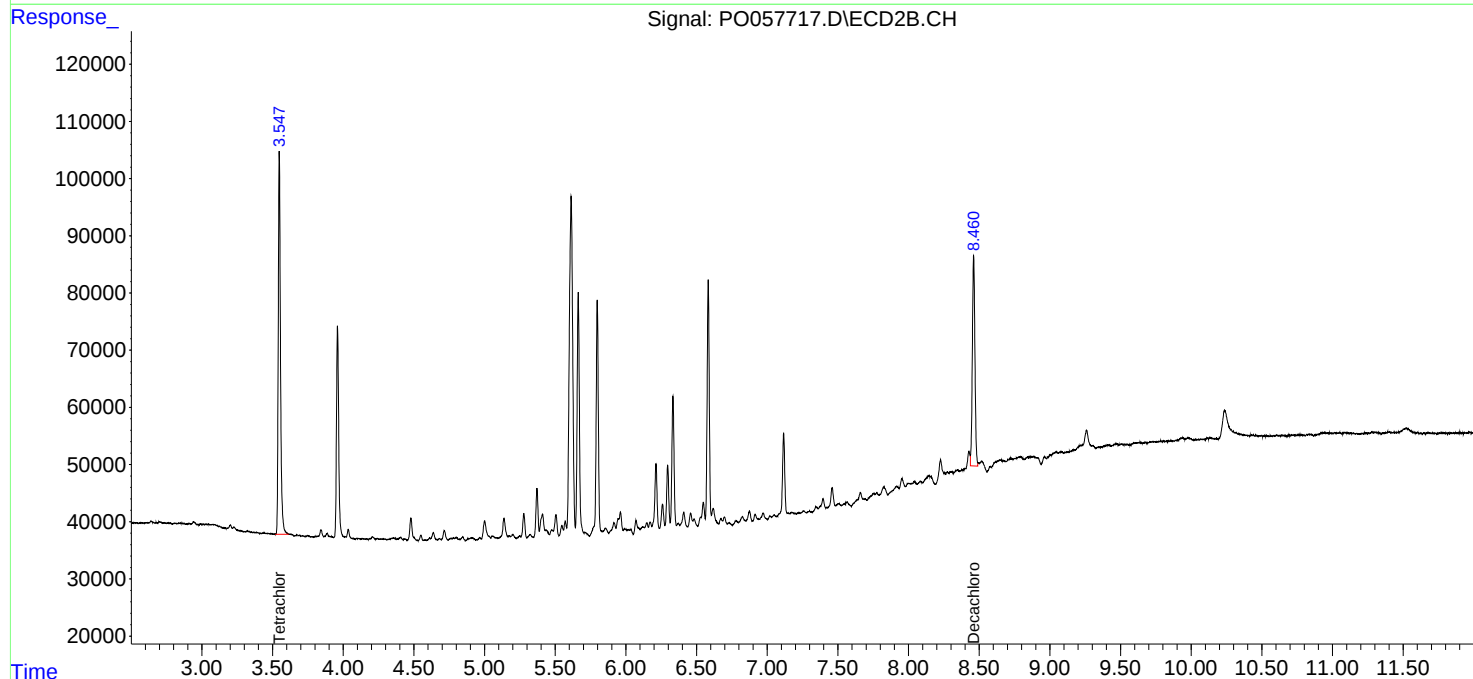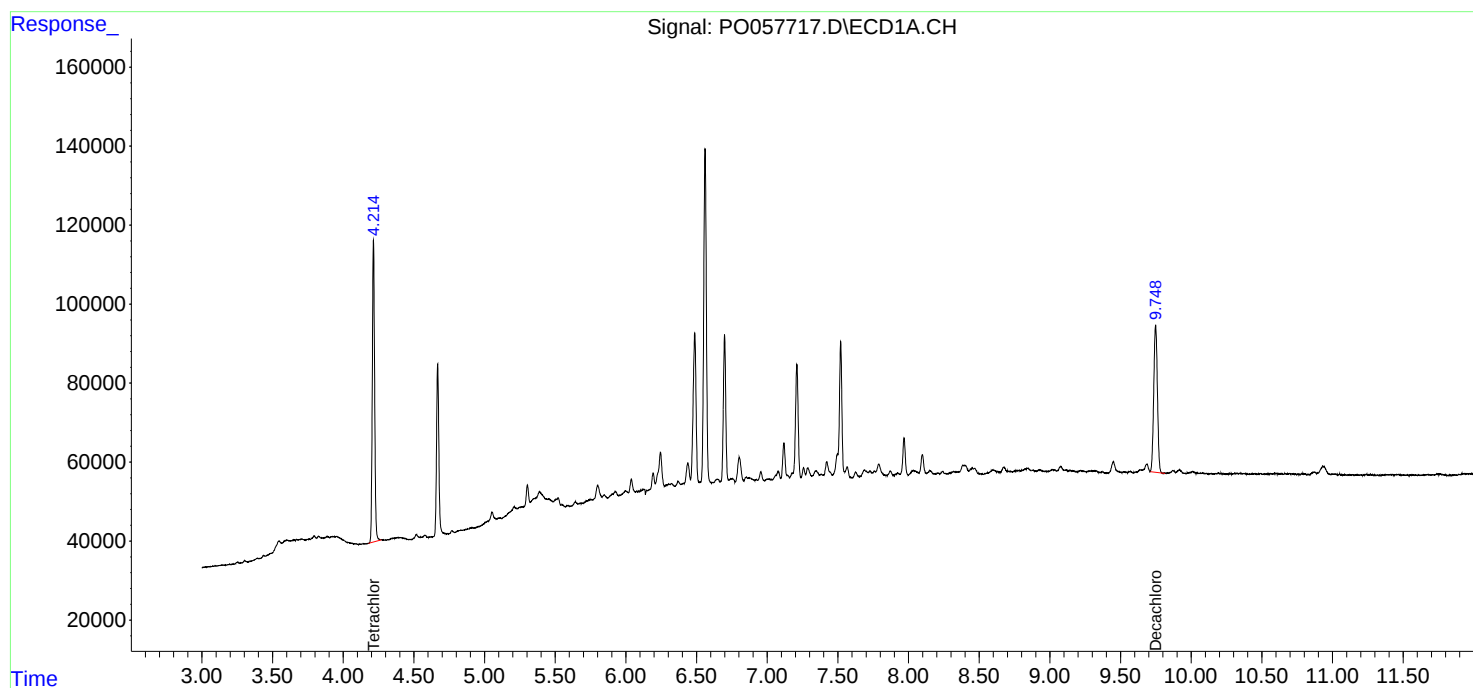

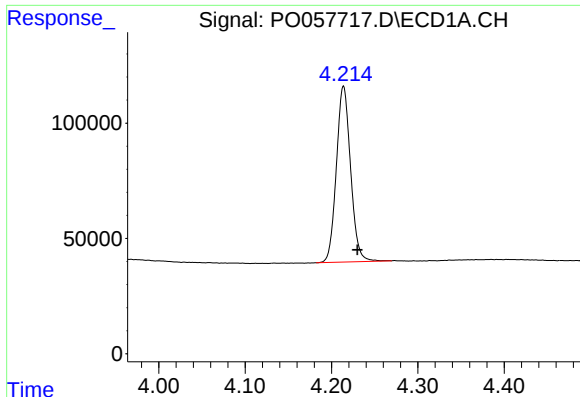


#1 Tetrachloro-m-xylene

R.T.: 4.214 min
Delta R.T.: -0.016 min
Response: 871350
Conc: 22.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
HL4-1(3-3.5)


Manual Integrations
APPROVED

Ankita
7/8/2019 11:09:37 AM

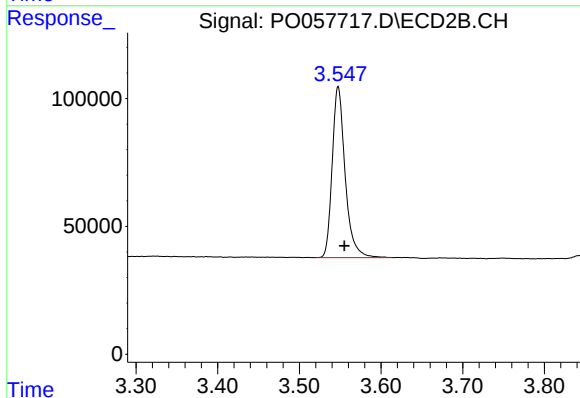


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.008 min
Response: 736213
Conc: 20.94 ng/ml

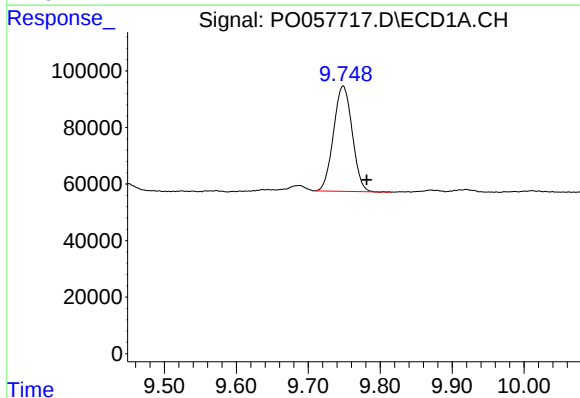

#2 Decachlorobiphenyl

R.T.: 9.748 min
Delta R.T.: -0.033 min
Response: 672977
Conc: 11.97 ng/ml

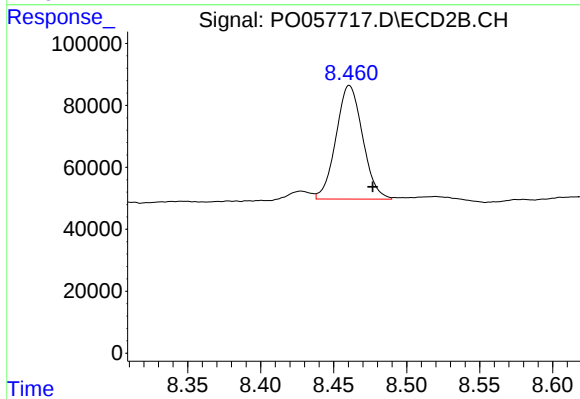

#2 Decachlorobiphenyl

R.T.: 8.460 min
Delta R.T.: -0.017 min
Response: 465255
Conc: 12.44 ng/ml m