

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070819\
 Data File : P0057733.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jul 2019 12:00
 Operator : SM/SJ
 Sample : K3653-10RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HL2-1(2.5-3)RE

Manual Integrations
 APPROVED

Ankita
 7/9/2019 9:35:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 12:58:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.214	3.547	1034973	919958	26.348	26.163
2) SA Decachlor...	9.744	8.458	2447130	1631484	43.518m	43.615

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070819\
Data File : PO057733.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jul 2019 12:00
Operator : SM/SJ
Sample : K3653-10RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HL2-1(2.5-3)RE


Manual Integrations
APPROVED

Ankita
7/9/2019 9:35:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 12:58:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

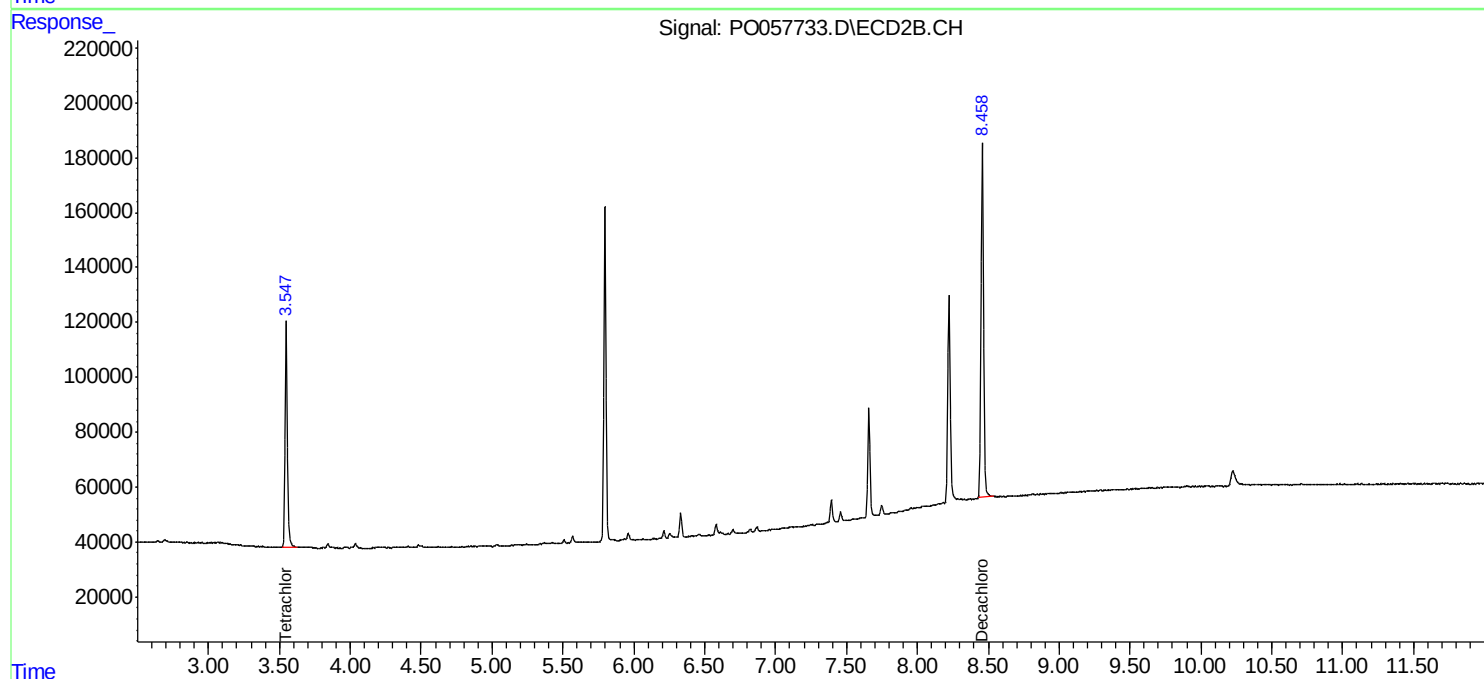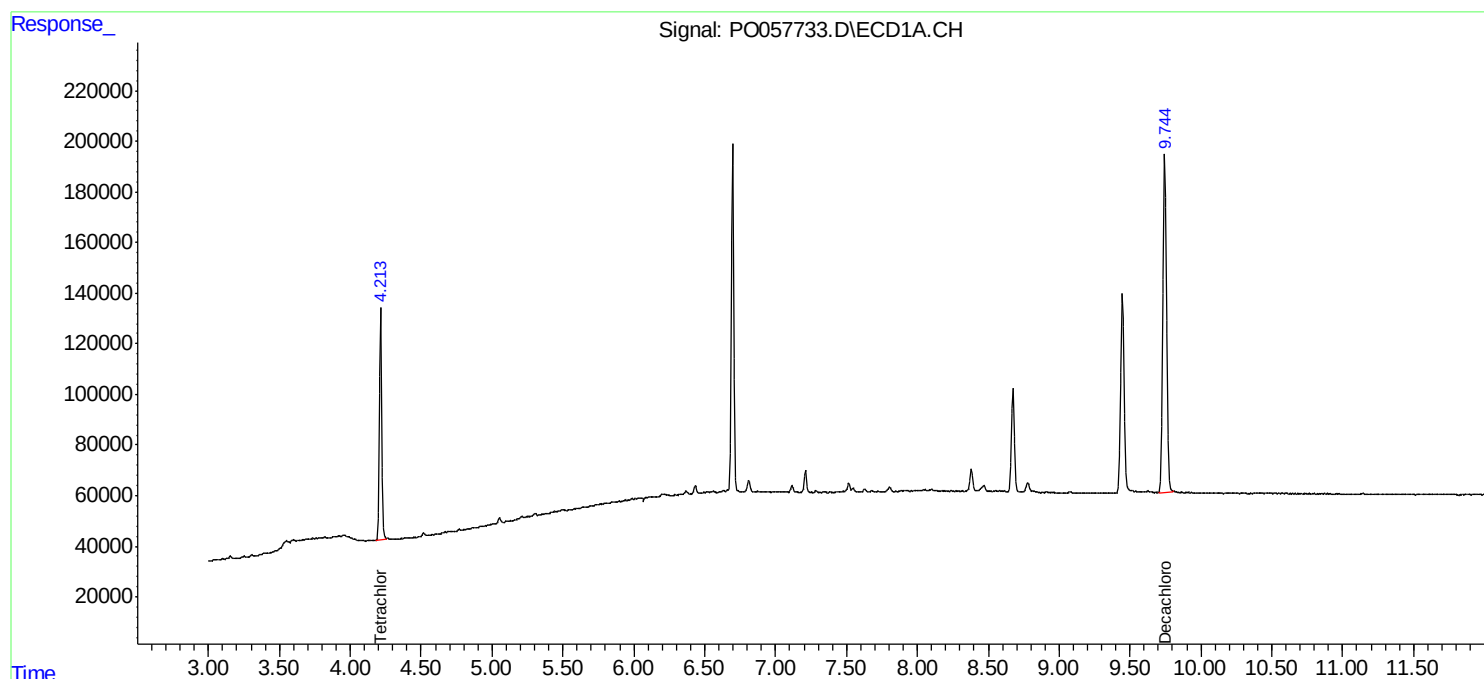

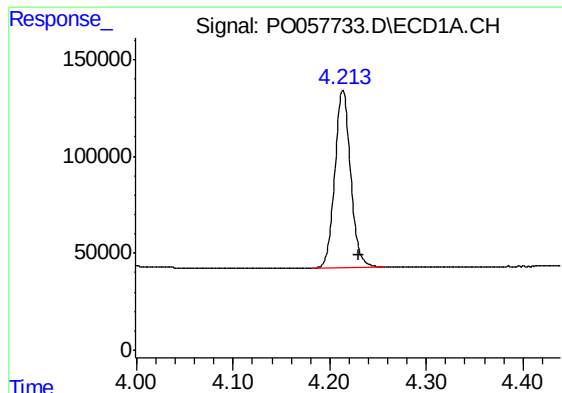


#1 Tetrachloro-m-xylene

R.T.: 4.214 min
Delta R.T.: -0.016 min
Response: 1034973
Conc: 26.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
HL2-1(2.5-3)RE


Manual Integrations
APPROVED

Ankita
7/9/2019 9:35:51 AM

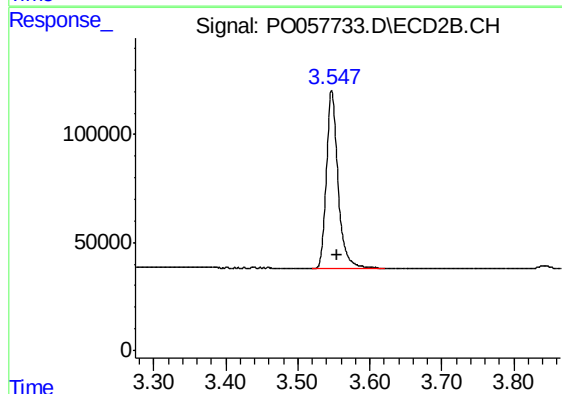


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: -0.008 min
Response: 919958
Conc: 26.16 ng/ml

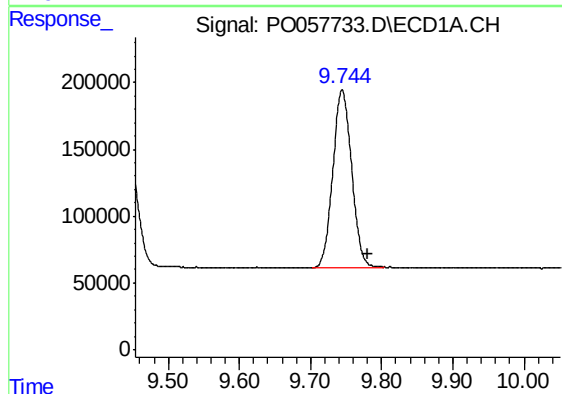

#2 Decachlorobiphenyl

R.T.: 9.744 min
Delta R.T.: -0.037 min
Response: 2447130
Conc: 43.52 ng/ml m

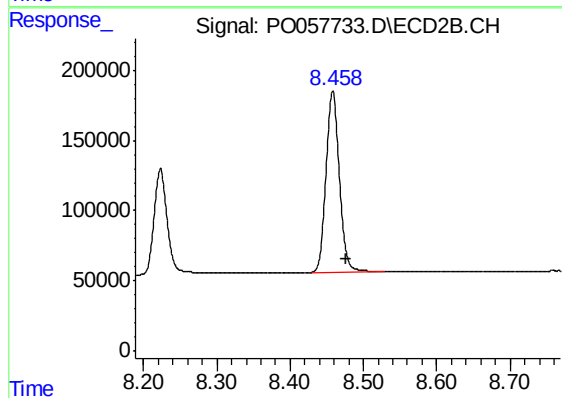

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.019 min
Response: 1631484
Conc: 43.61 ng/ml