

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070819\
 Data File : P0057748.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jul 2019 18:22
 Operator : SM/SJ
 Sample : PB121184BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB121184BL

Manual Integrations
 APPROVED

Ankita
 7/9/2019 9:36:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 01:19:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.211	3.546	794114	718527	20.216	20.434
2)	SA Decachlor...	9.742	8.458	1284917	848384	22.850m	22.680

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070819\
Data File : PO057748.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jul 2019 18:22
Operator : SM/SJ
Sample : PB121184BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB121184BL


Manual Integrations
APPROVED

Ankita
7/9/2019 9:36:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 01:19:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

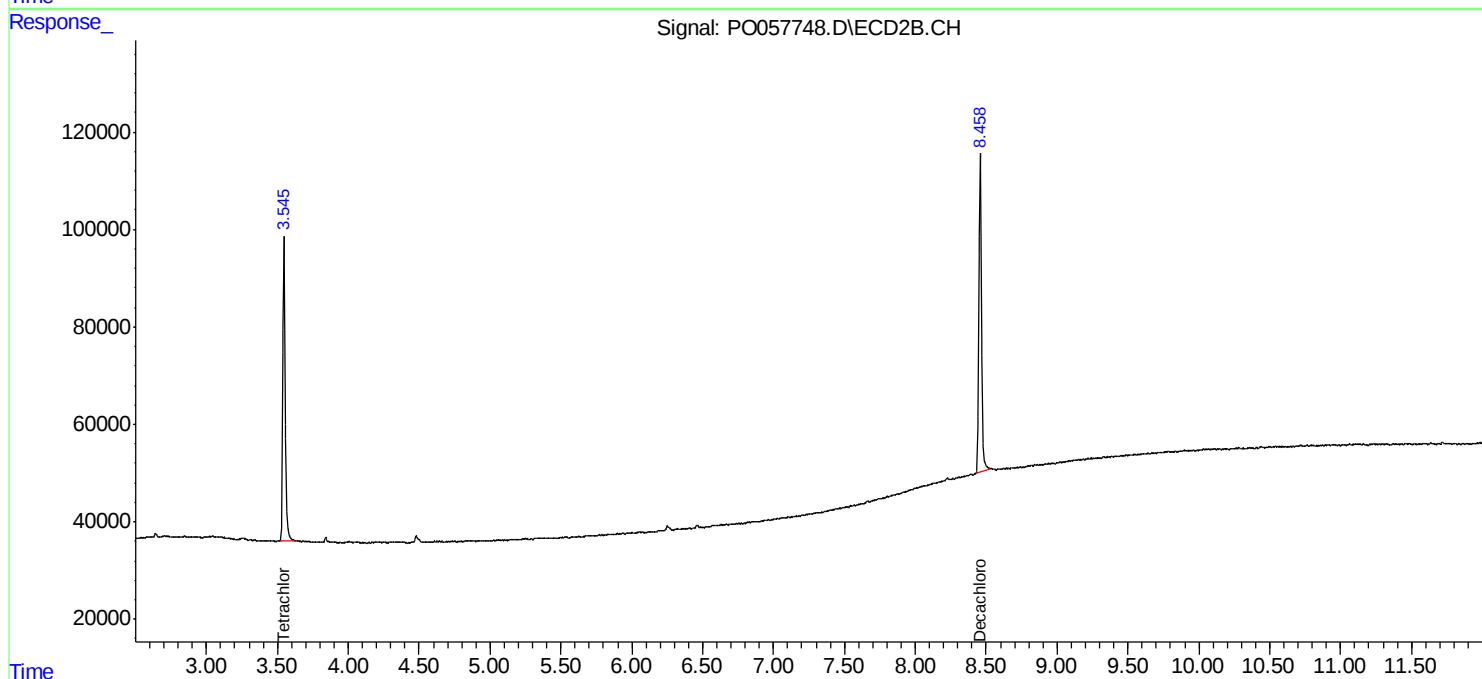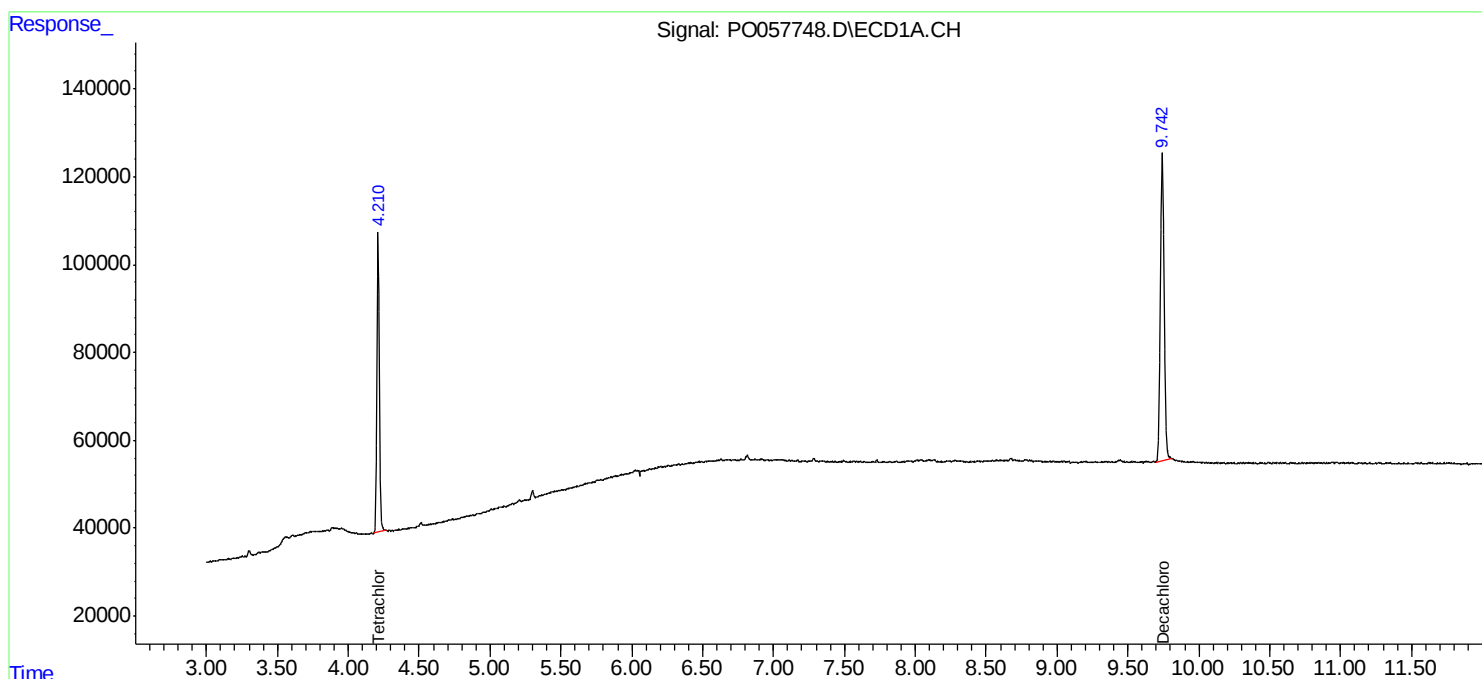

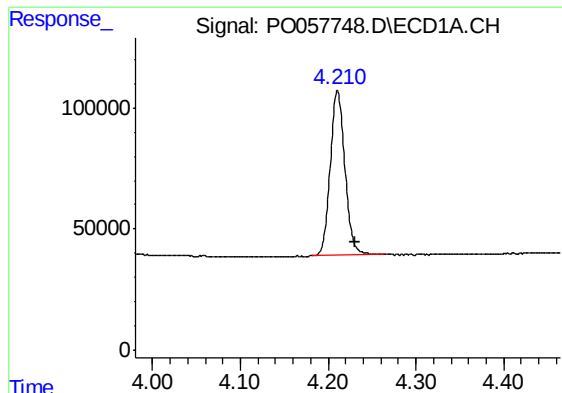


#1 Tetrachloro-m-xylene

R.T.: 4.211 min
Delta R.T.: -0.019 min
Response: 794114
Conc: 20.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB121184BL


Manual Integrations
APPROVED

Ankita
7/9/2019 9:36:36 AM

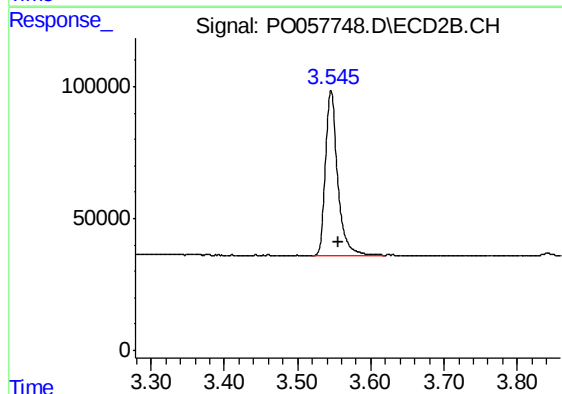


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.010 min
Response: 718527
Conc: 20.43 ng/ml

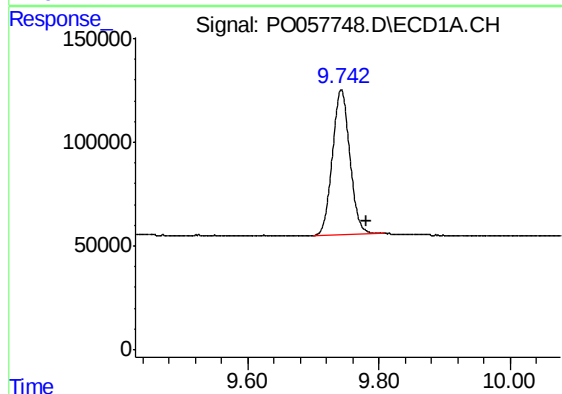

#2 Decachlorobiphenyl

R.T.: 9.742 min
Delta R.T.: -0.039 min
Response: 1284917
Conc: 22.85 ng/ml m

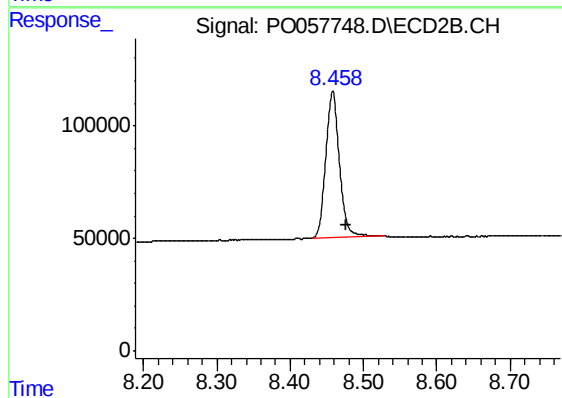

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.019 min
Response: 848384
Conc: 22.68 ng/ml