

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070819\
 Data File : P0057751.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jul 2019 19:13
 Operator : SM/SJ
 Sample : K3636-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP19-MMW0018B

Manual Integrations
 APPROVED

Ankita
 7/9/2019 9:36:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 01:21:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.211	3.548	660286	608399	16.809	17.302
2) SA Decachlor...	9.743	8.458	1035082	655951	18.407m	17.536

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070819\
Data File : PO057751.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jul 2019 19:13
Operator : SM/SJ
Sample : K3636-11
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP19-MMW0018B


Manual Integrations
APPROVED

Ankita
7/9/2019 9:36:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 01:21:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

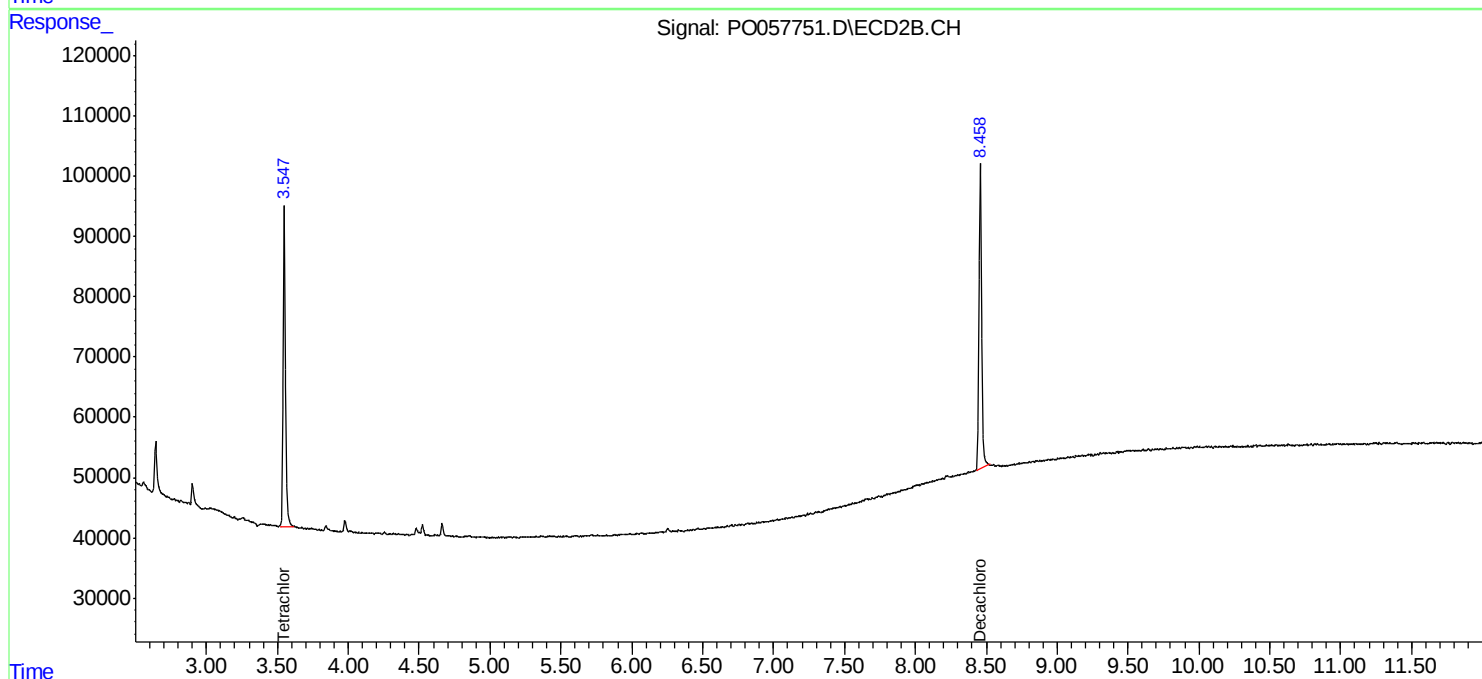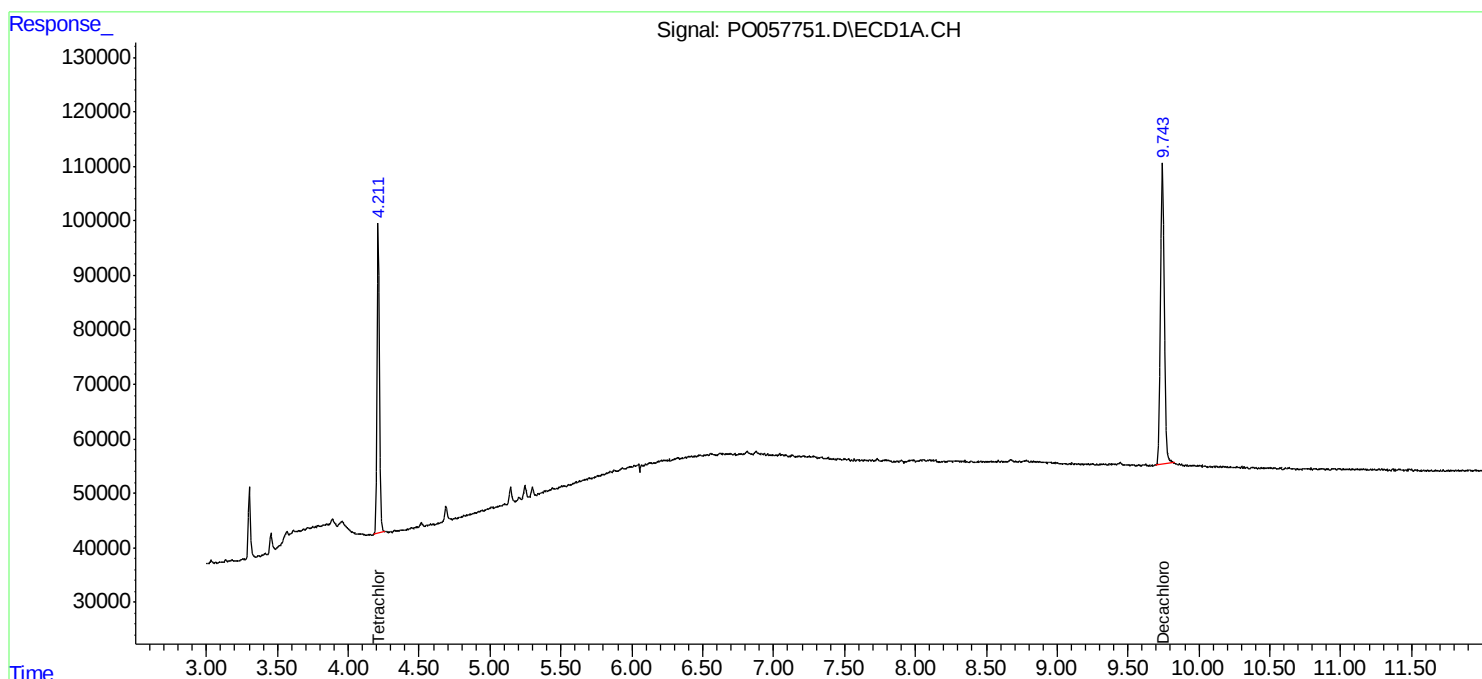

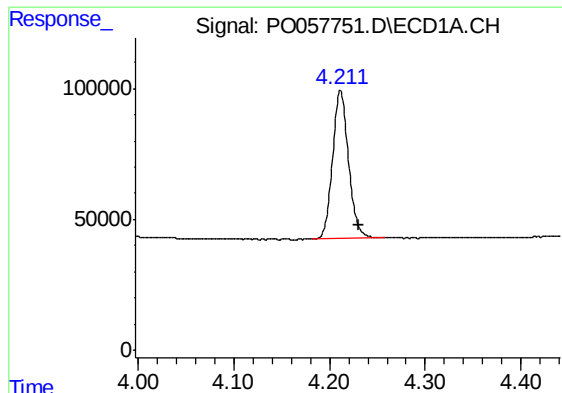


#1 Tetrachloro-m-xylene

R.T.: 4.211 min
Delta R.T.: -0.019 min
Response: 660286
Conc: 16.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP19-MMW0018B


Manual Integrations
APPROVED

Ankita
7/9/2019 9:36:59 AM

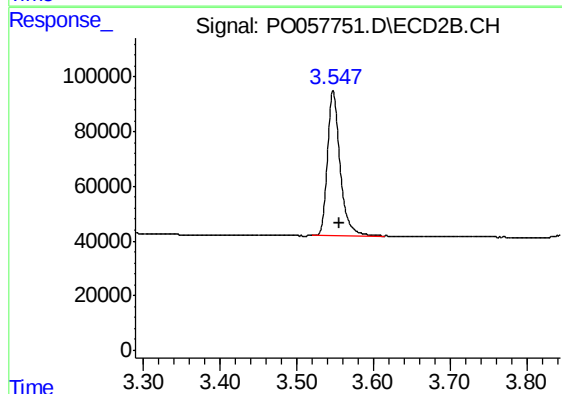


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.008 min
Response: 608399
Conc: 17.30 ng/ml

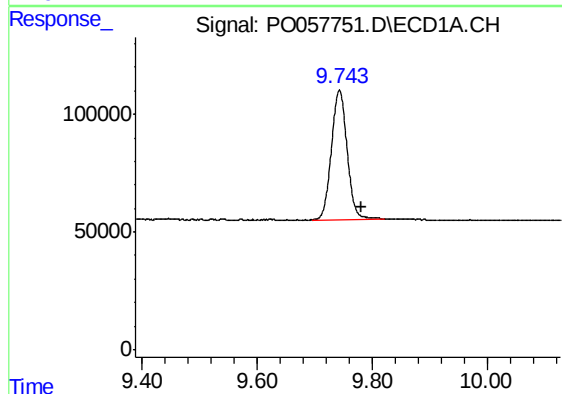

#2 Decachlorobiphenyl

R.T.: 9.743 min
Delta R.T.: -0.038 min
Response: 1035082
Conc: 18.41 ng/ml m

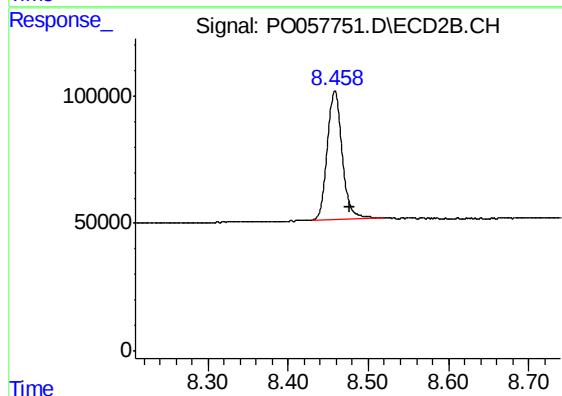

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.019 min
Response: 655951
Conc: 17.54 ng/ml