

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0070918\
Data File : P0046469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2018 11:07
Operator : SM/UA
Sample : J3868-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-7-D

Manual Integrations
APPROVED

Sohil
7/11/2018 11:30:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 11:21:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 07:25:43 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.213	3.540	6256810	5854242	26.179	27.562
2) SA Decachlor...	9.750	8.475	3928880	3783656	20.617m	19.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0070918\
Data File : P0046469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2018 11:07
Operator : SM/UA
Sample : J3868-07
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-7-D


Manual Integrations
APPROVED

Sohil
7/11/2018 11:30:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 11:21:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 07:25:43 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

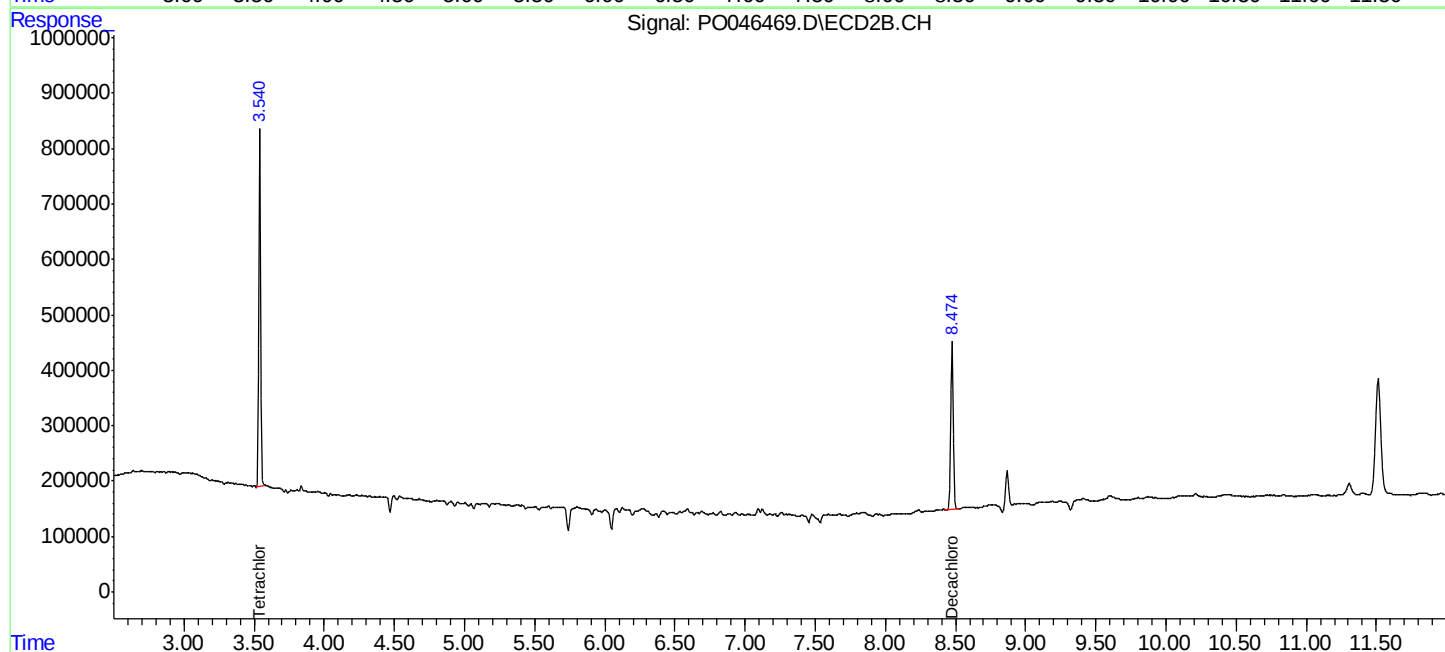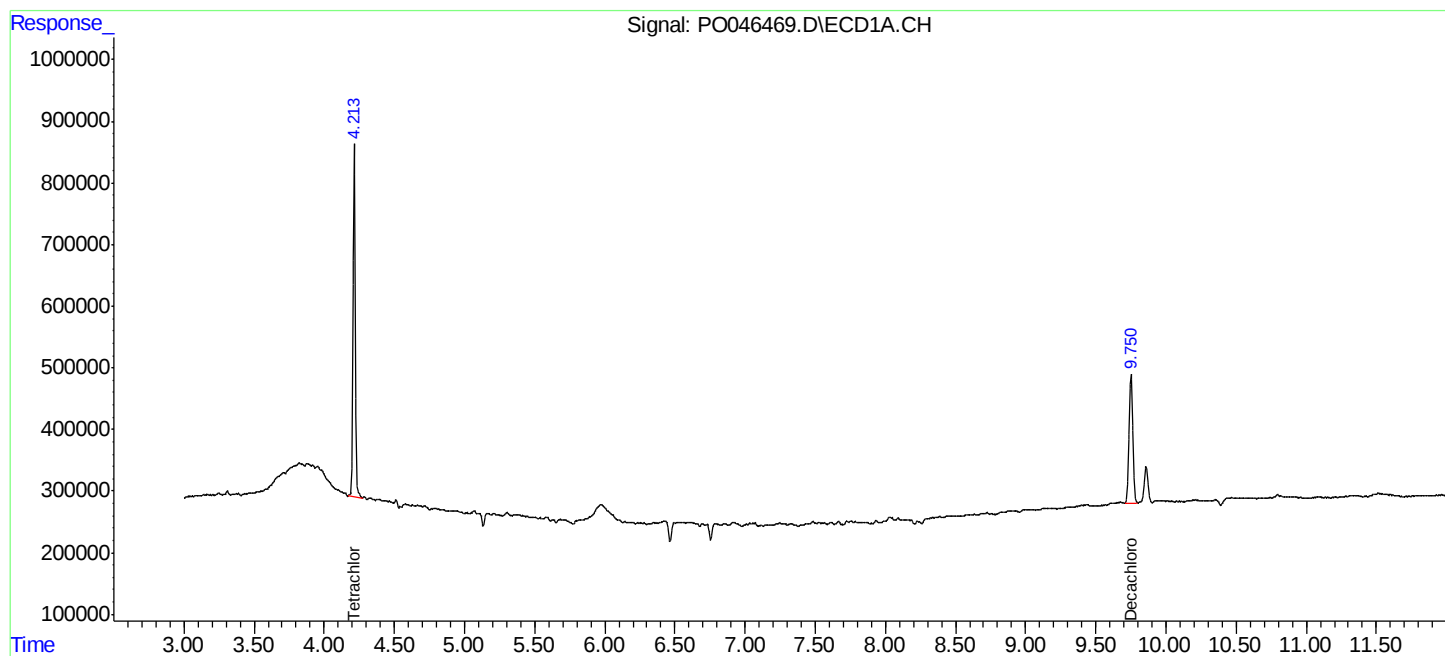

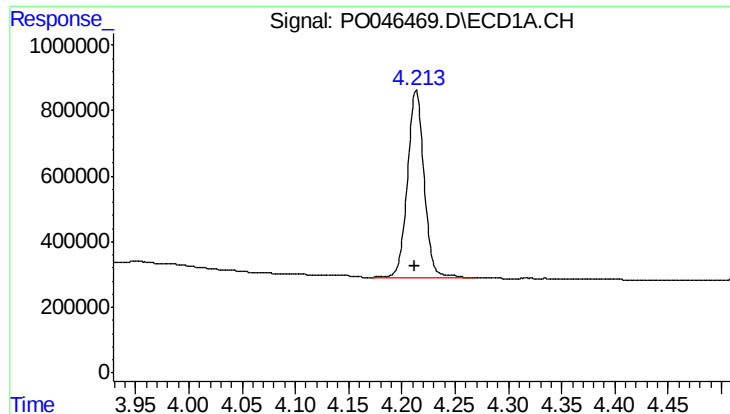


#1 Tetrachloro-m-xylene

R.T.: 4.213 min
Delta R.T.: 0.001 min
Response: 6256810
Conc: 26.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-7-D


Manual Integrations
APPROVED

Sohil
7/11/2018 11:30:04 AM

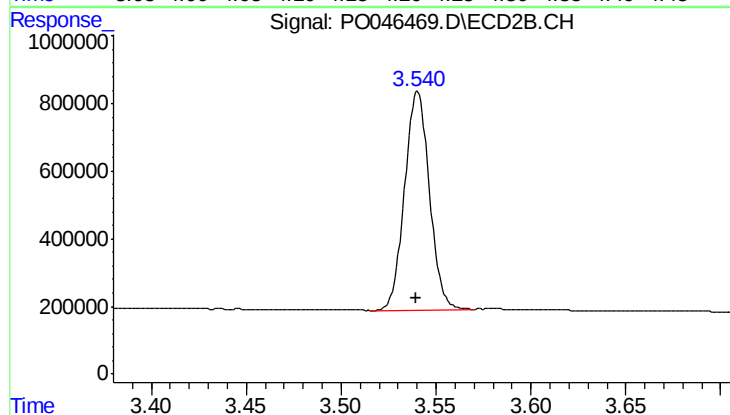


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 5854242
Conc: 27.56 ng/ml

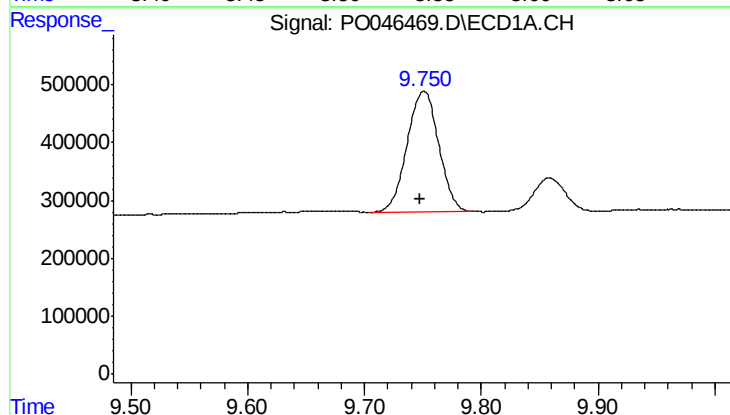

#2 Decachlorobiphenyl

R.T.: 9.750 min
Delta R.T.: 0.002 min
Response: 3928880
Conc: 20.62 ng/ml m

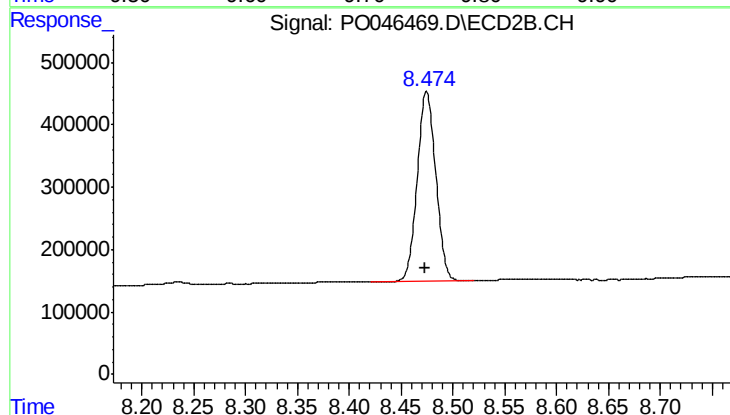

#2 Decachlorobiphenyl

R.T.: 8.475 min
Delta R.T.: 0.001 min
Response: 3783656
Conc: 19.51 ng/ml