

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071019\
 Data File : P0057769.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jul 2019 14:33
 Operator : SM/SJ
 Sample : PB121227BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB121227BL

Manual Integrations
 APPROVED

Ankita
 7/10/2019 8:40:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 02:04:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.209	3.545	765752	693246	19.494	19.715
2)	SA Decachlor...	9.740	8.456	1226305	769416	21.808m	20.569

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071019\
Data File : PO057769.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2019 14:33
Operator : SM/SJ
Sample : PB121227BL
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB121227BL


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 02:04:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

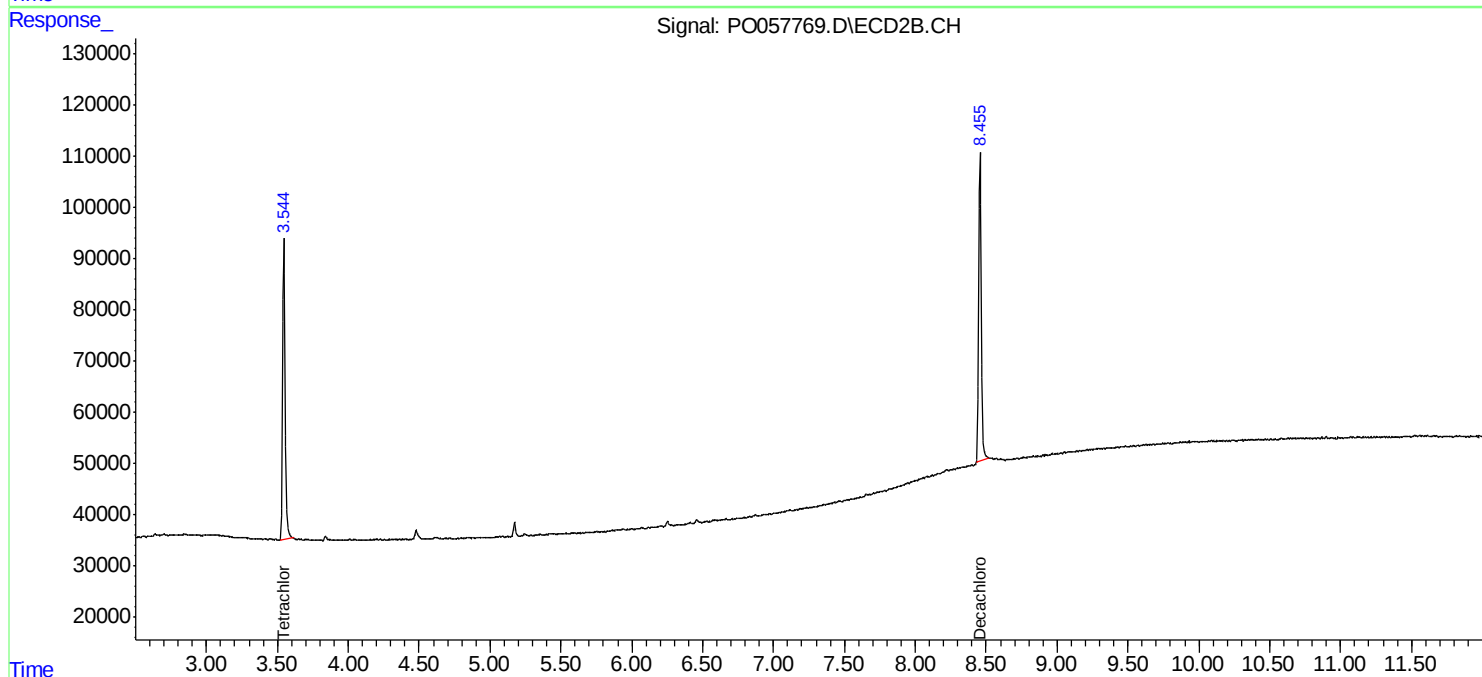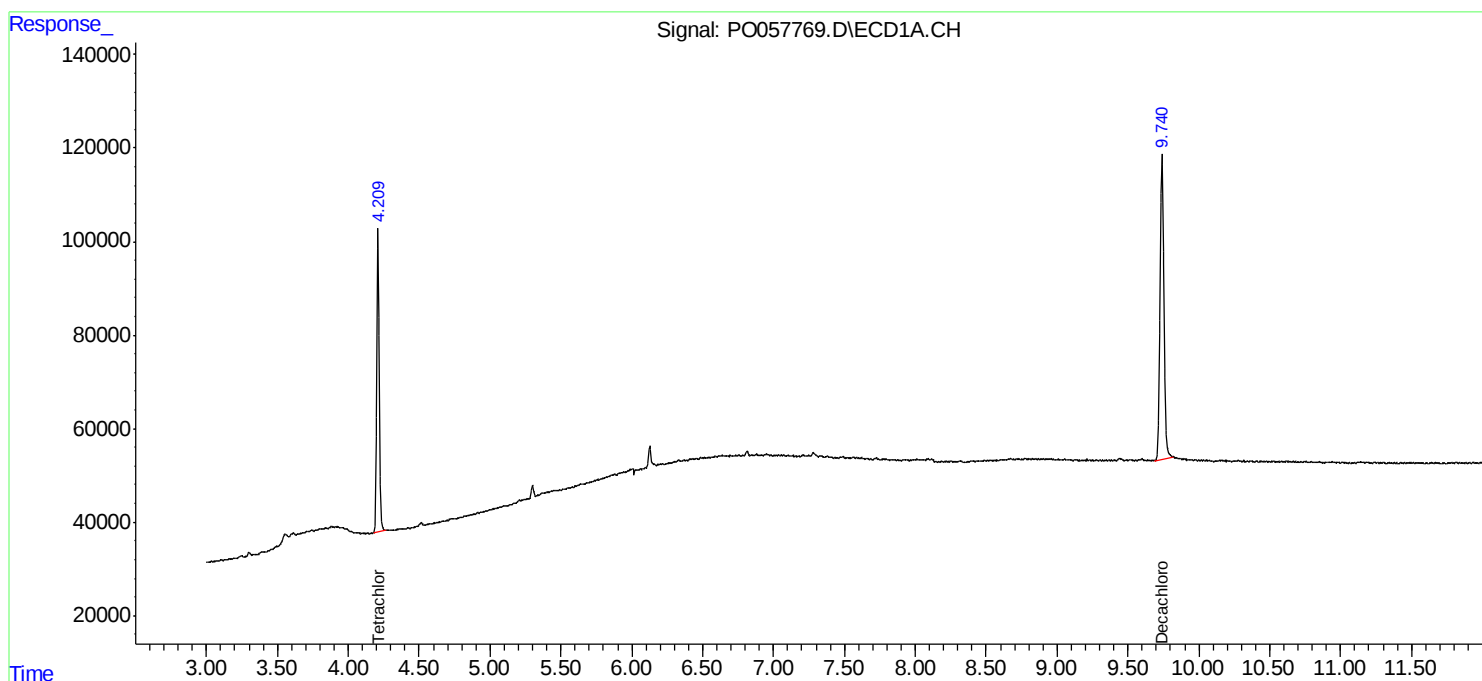

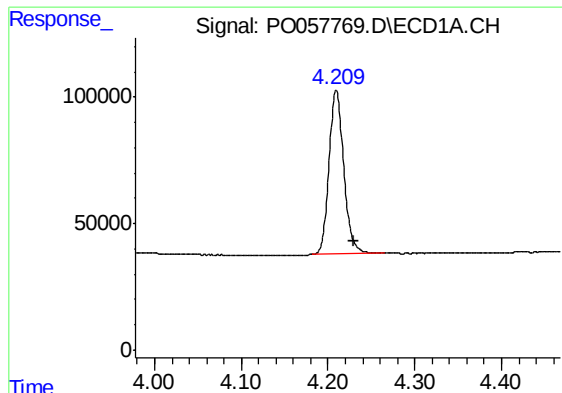


#1 Tetrachloro-m-xylene

R.T.: 4.209 min
Delta R.T.: -0.021 min
Response: 765752
Conc: 19.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB121227BL


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:04 AM

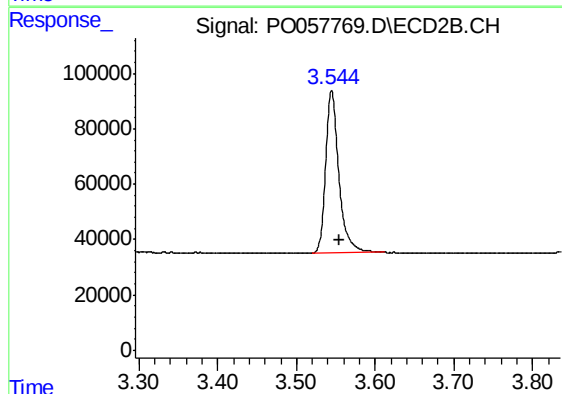


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.011 min
Response: 693246
Conc: 19.72 ng/ml

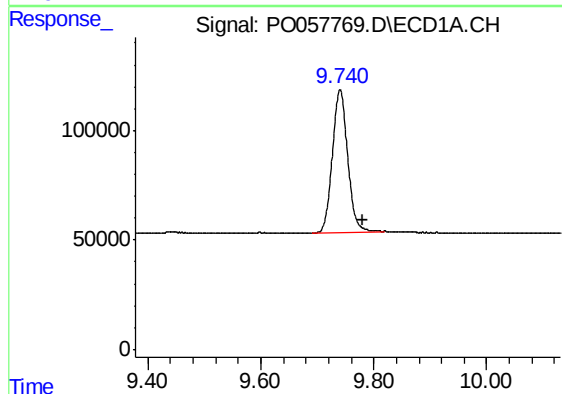

#2 Decachlorobiphenyl

R.T.: 9.740 min
Delta R.T.: -0.041 min
Response: 1226305
Conc: 21.81 ng/ml m

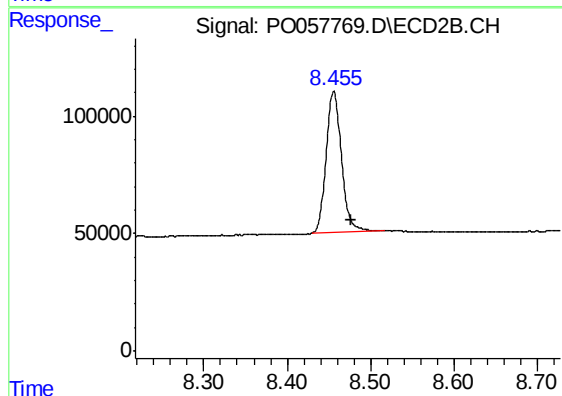

#2 Decachlorobiphenyl

R.T.: 8.456 min
Delta R.T.: -0.021 min
Response: 769416
Conc: 20.57 ng/ml