

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071019\
 Data File : P0057778.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2019 1:30
 Operator : SM/SJ
 Sample : K3697-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RBR-200035

Manual Integrations
 APPROVED

Ankita
 7/10/2019 8:40:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:54:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.227	3.546	737716	696300	18.780	19.802
2) SA Decachlor...	9.758	8.443	1588234	1052606	28.244	28.139m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071019\
Data File : PO057778.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2019 1:30
Operator : SM/SJ
Sample : K3697-04
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RBR-200035


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:54:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

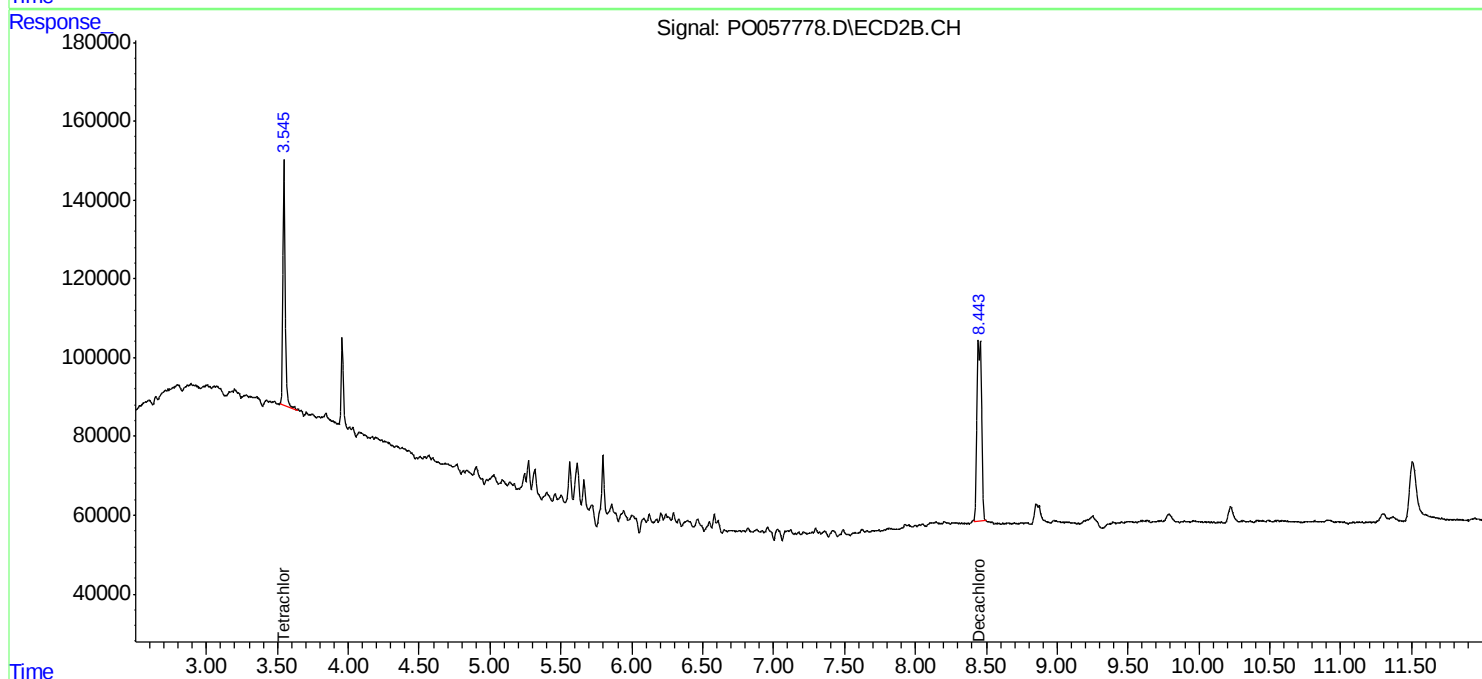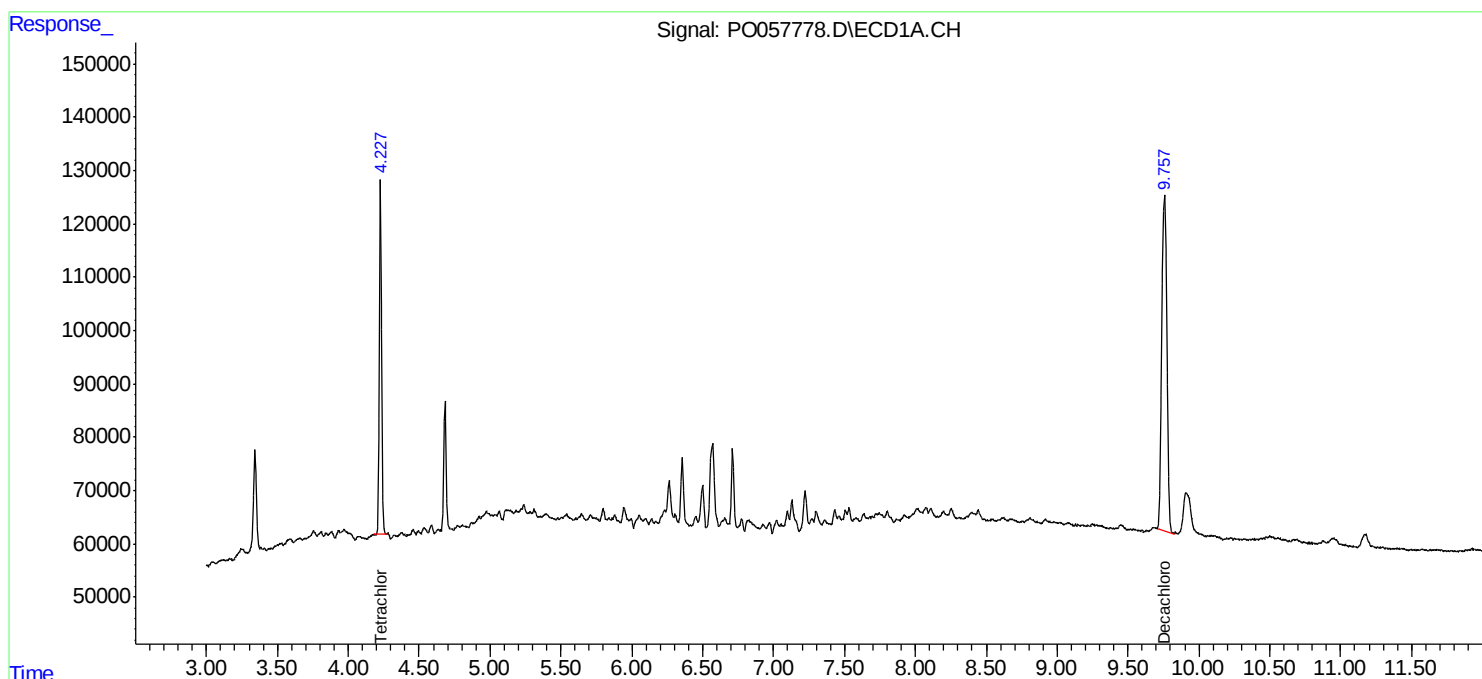

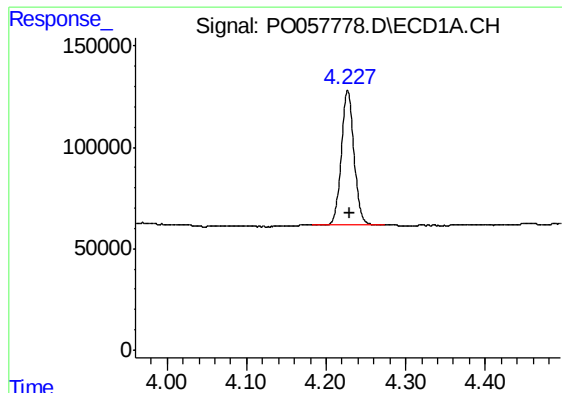


#1 Tetrachloro-m-xylene

R.T.: 4.227 min
Delta R.T.: -0.003 min
Response: 737716
Conc: 18.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
RBR-200035


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:20 AM

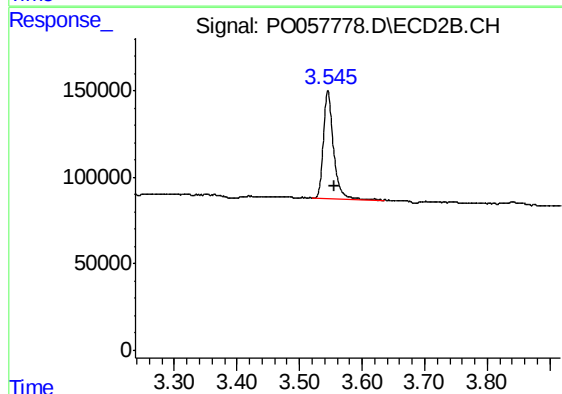


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.010 min
Response: 696300
Conc: 19.80 ng/ml

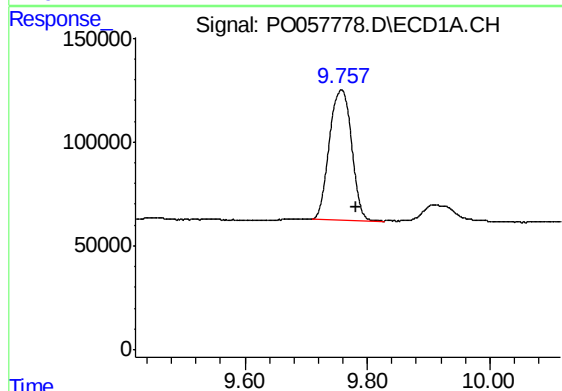

#2 Decachlorobiphenyl

R.T.: 9.758 min
Delta R.T.: -0.024 min
Response: 1588234
Conc: 28.24 ng/ml

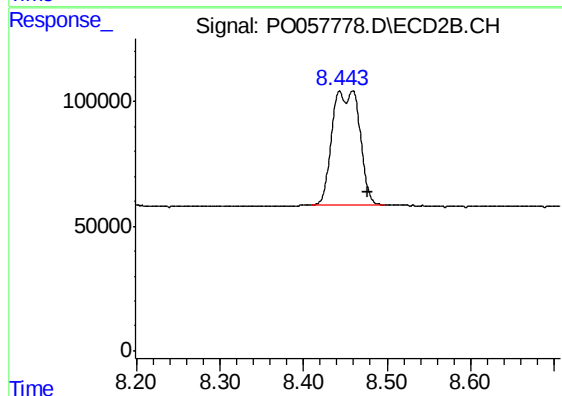

#2 Decachlorobiphenyl

R.T.: 8.443 min
Delta R.T.: -0.034 min
Response: 1052606
Conc: 28.14 ng/ml m