

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071019\
 Data File : P0057779.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2019 1:46
 Operator : SM/SJ
 Sample : K3698-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 06-A-06-B-06-C

Manual Integrations
 APPROVED

Ankita
 7/10/2019 8:40:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:55:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.212	3.547	885786	717794	22.550	20.413
2)	SA Decachlor...	9.742	8.453	1524247	833538	27.106m	22.283m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071019\
Data File : P0057779.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2019 1:46
Operator : SM/SJ
Sample : K3698-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:55:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

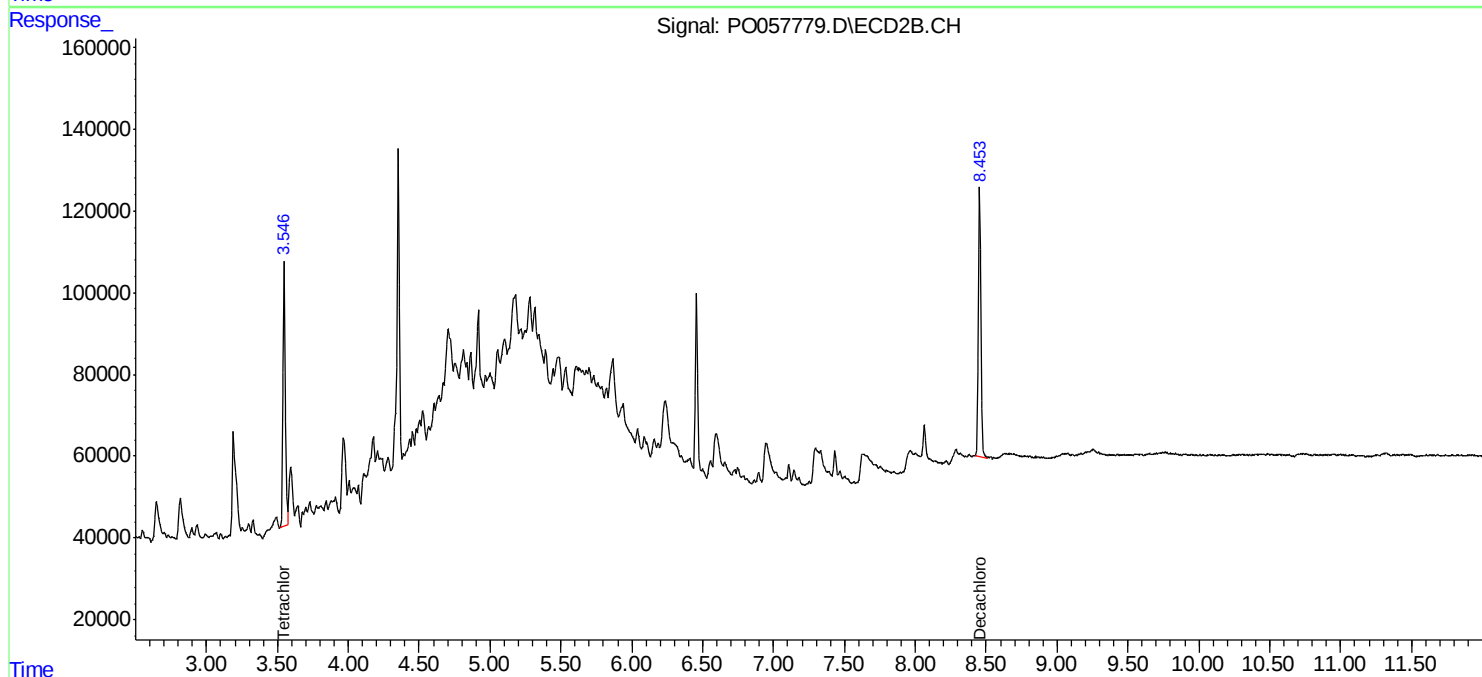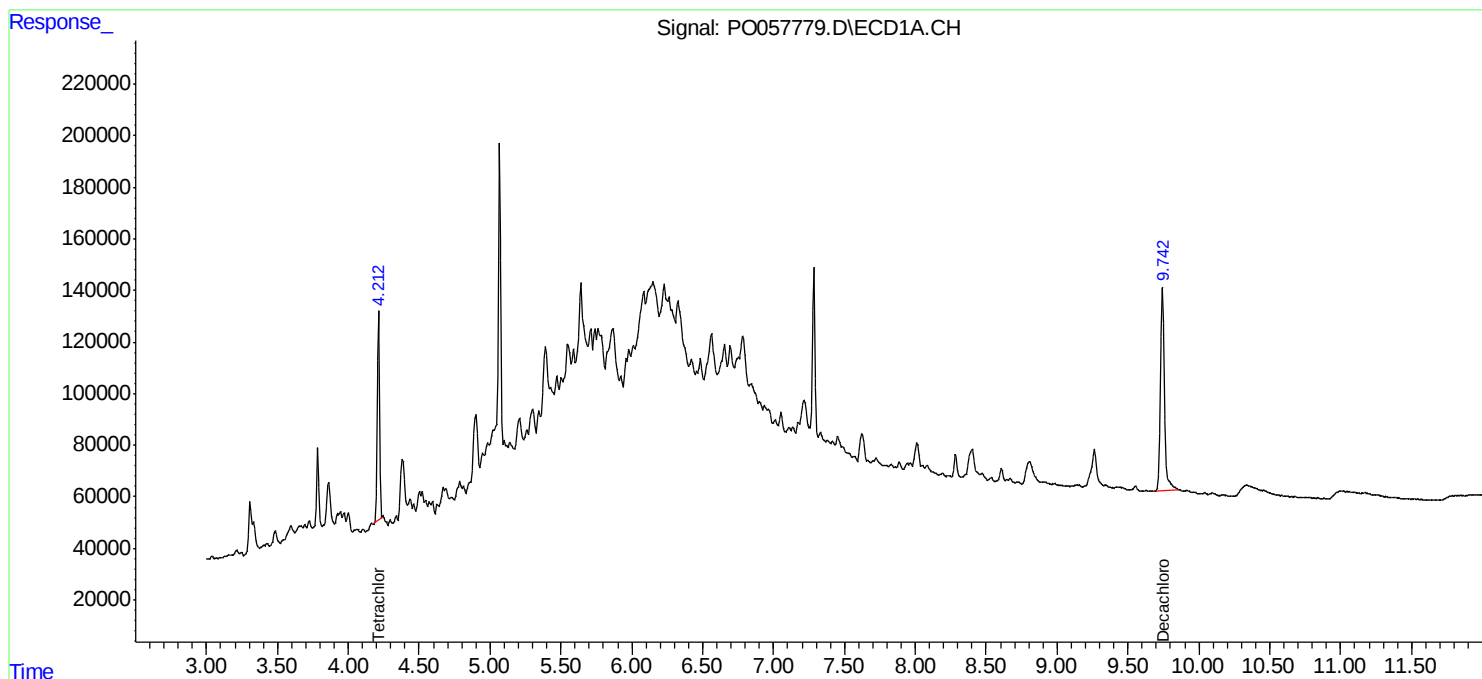

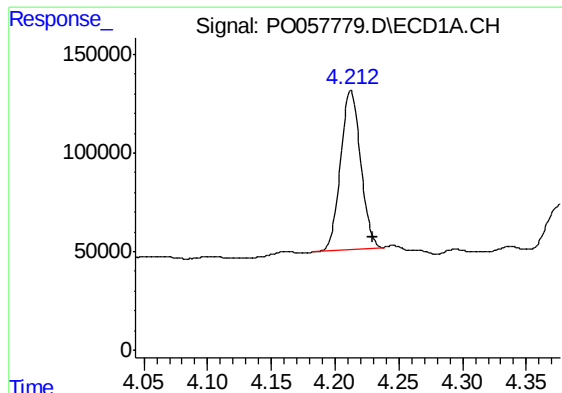


#1 Tetrachloro-m-xylene

R.T.: 4.212 min
Delta R.T.: -0.018 min
Response: 885786
Conc: 22.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:21 AM

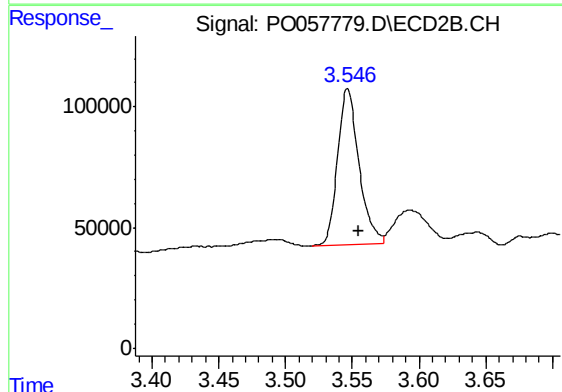


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: -0.009 min
Response: 717794
Conc: 20.41 ng/ml

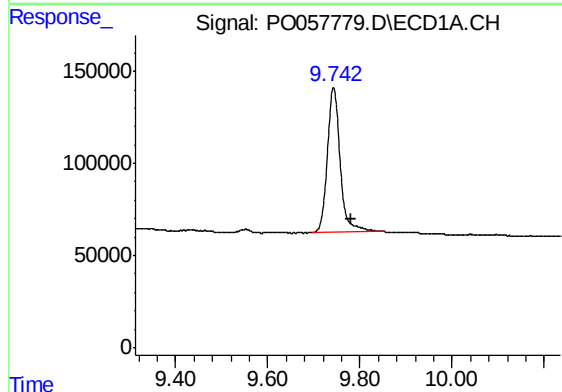

#2 Decachlorobiphenyl

R.T.: 9.742 min
Delta R.T.: -0.039 min
Response: 1524247
Conc: 27.11 ng/ml m

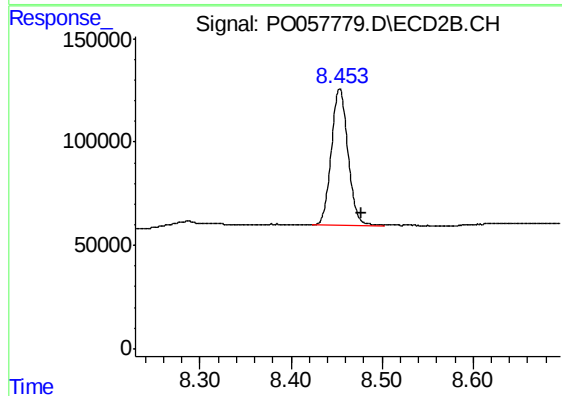

#2 Decachlorobiphenyl

R.T.: 8.453 min
Delta R.T.: -0.024 min
Response: 833538
Conc: 22.28 ng/ml m