

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071019\
 Data File : P0057780.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2019 2:03
 Operator : SM/SJ
 Sample : K3699-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-EF-01-014-ABCD

Manual Integrations
 APPROVED

Ankita
 7/10/2019 8:40:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:55:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.210	3.546	798622	708590	20.331m	20.152
2) SA Decachlor...	9.738	8.454	994172	647457	17.680m	17.309m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071019\
Data File : PO057780.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2019 2:03
Operator : SM/SJ
Sample : K3699-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-EF-01-014-ABCD


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:55:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

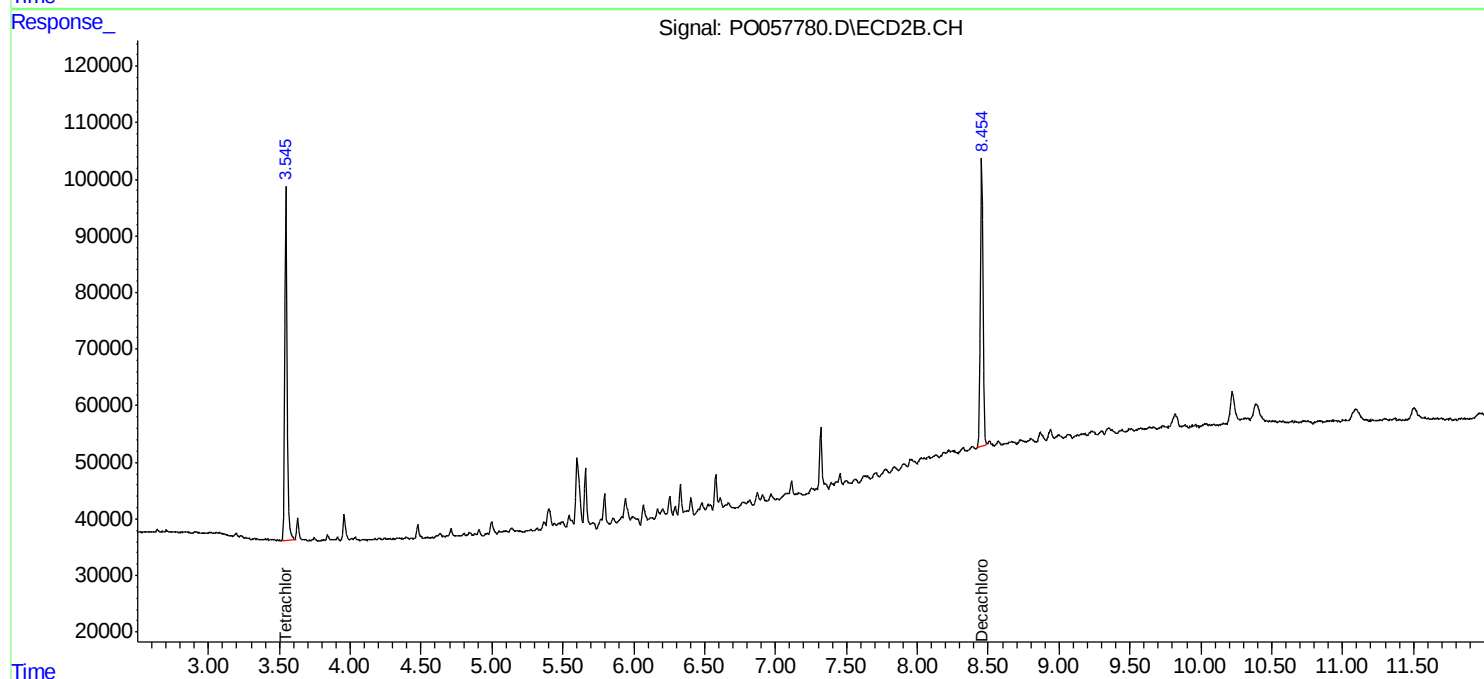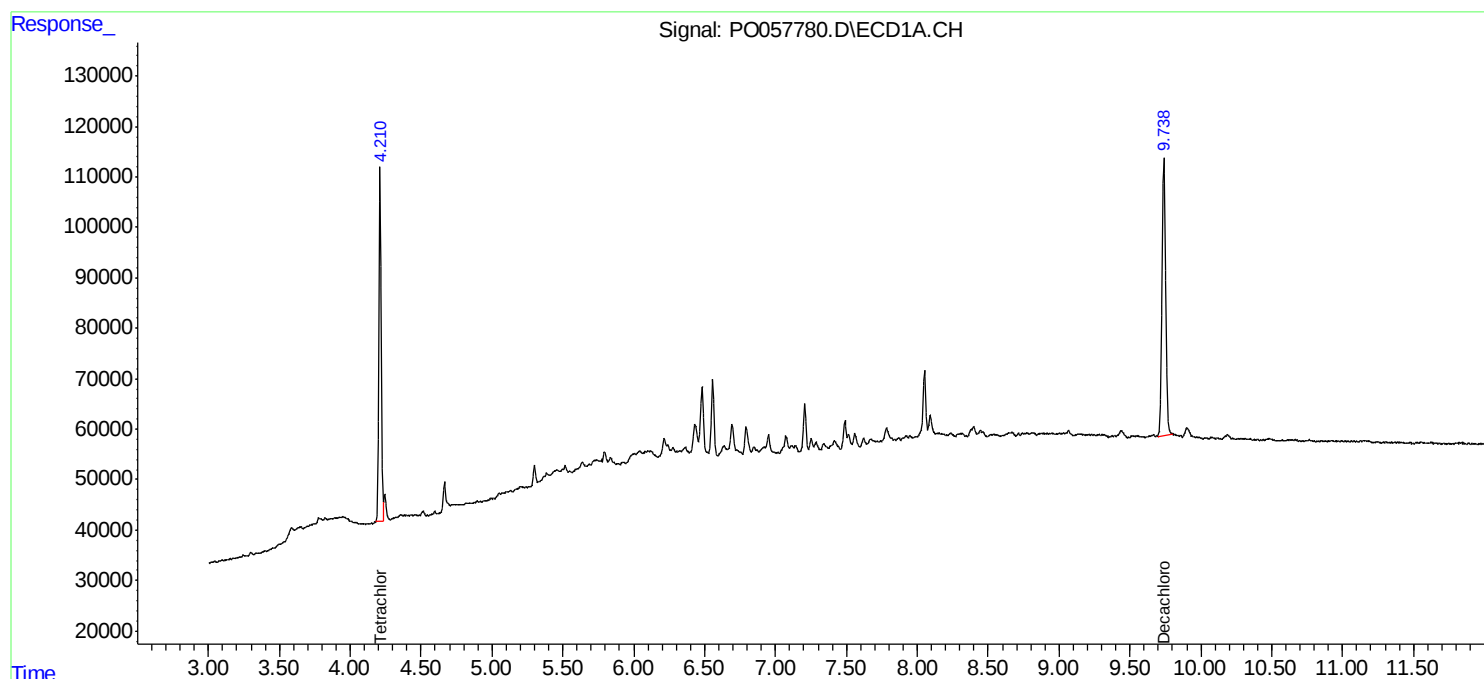

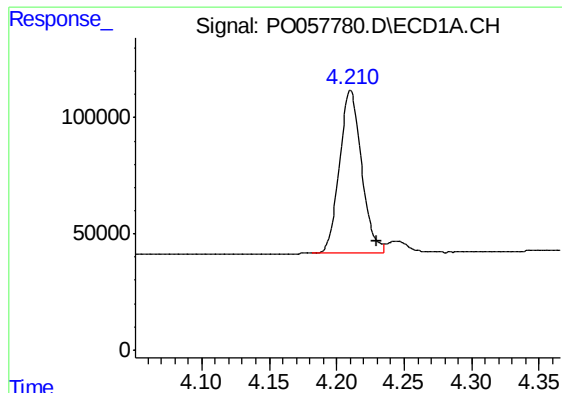


#1 Tetrachloro-m-xylene

R.T.: 4.210 min
Delta R.T.: -0.020 min
Response: 798622
Conc: 20.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-014-ABCD


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:22 AM

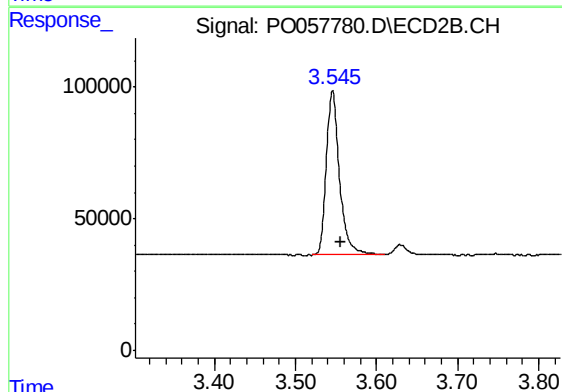


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.010 min
Response: 708590
Conc: 20.15 ng/ml

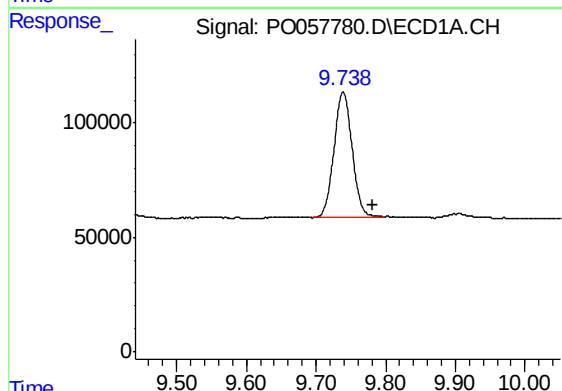

#2 Decachlorobiphenyl

R.T.: 9.738 min
Delta R.T.: -0.043 min
Response: 994172
Conc: 17.68 ng/ml m

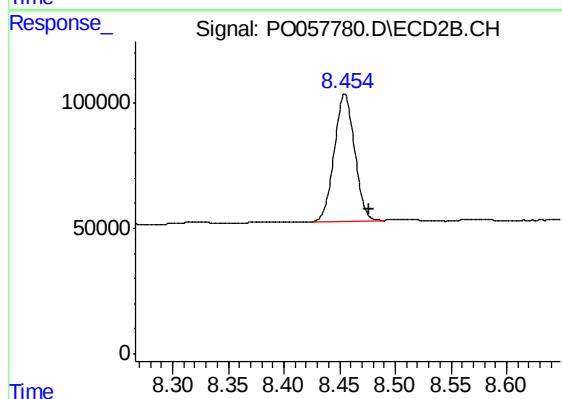

#2 Decachlorobiphenyl

R.T.: 8.454 min
Delta R.T.: -0.023 min
Response: 647457
Conc: 17.31 ng/ml m