

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071019\
 Data File : P0057782.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2019 2:37
 Operator : SM/SJ
 Sample : K3703-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-EF-01-015-ABCD

Manual Integrations
 APPROVED

Ankita
 7/10/2019 8:40:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:56:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.209	3.545	881325	775895	22.436m	22.066
2) SA Decachlor...	9.736	8.453	1075088	693466	19.118m	18.538

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071019\
Data File : PO057782.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2019 2:37
Operator : SM/SJ
Sample : K3703-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-EF-01-015-ABCD


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:56:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

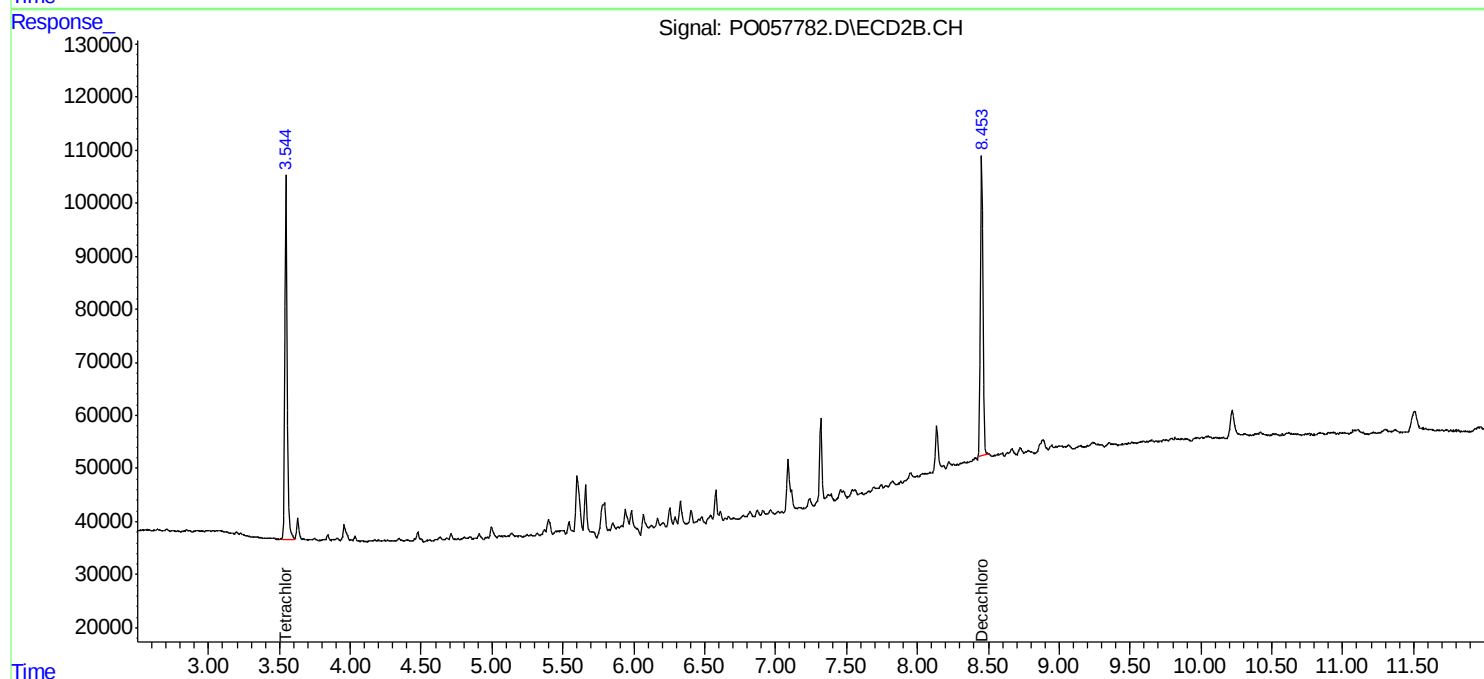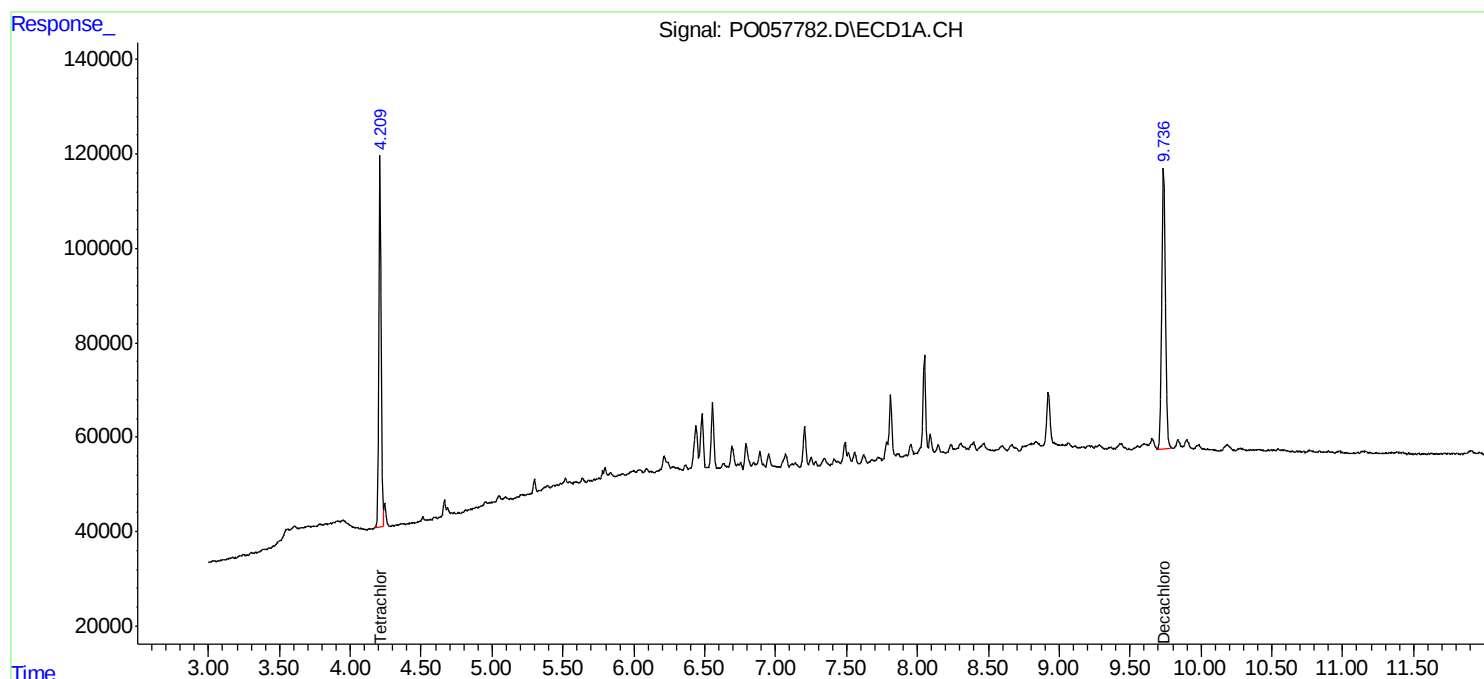

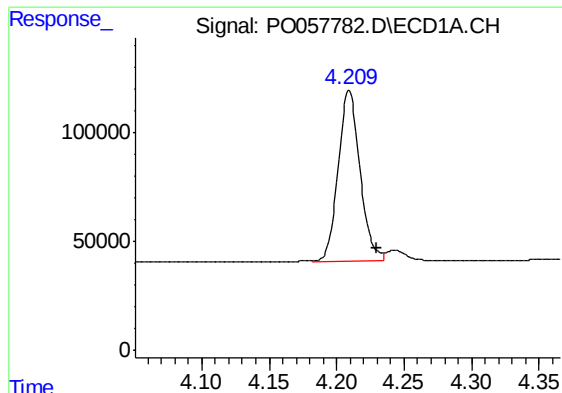


#1 Tetrachloro-m-xylene

R.T.: 4.209 min
Delta R.T.: -0.021 min
Response: 881325
Conc: 22.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-015-ABCD


Manual Integrations
APPROVED

Ankita
7/10/2019 8:40:25 AM

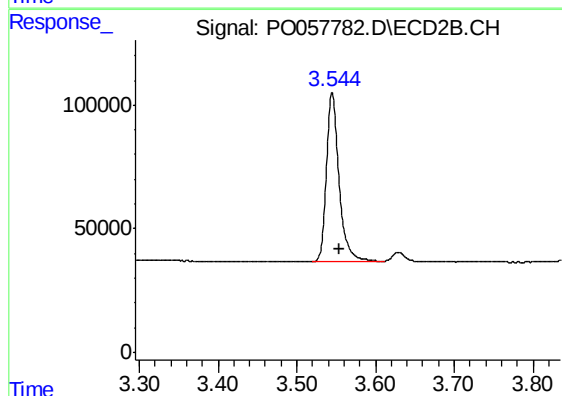


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.010 min
Response: 775895
Conc: 22.07 ng/ml

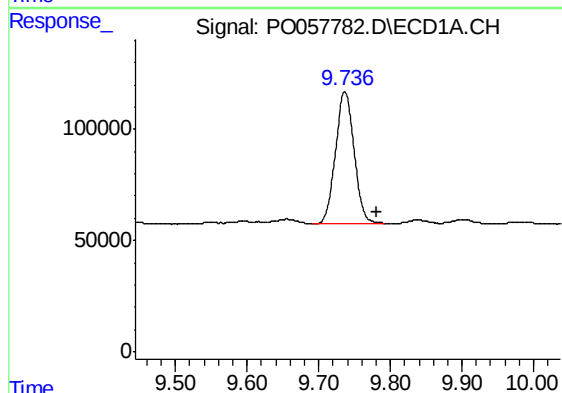

#2 Decachlorobiphenyl

R.T.: 9.736 min
Delta R.T.: -0.045 min
Response: 1075088
Conc: 19.12 ng/ml m

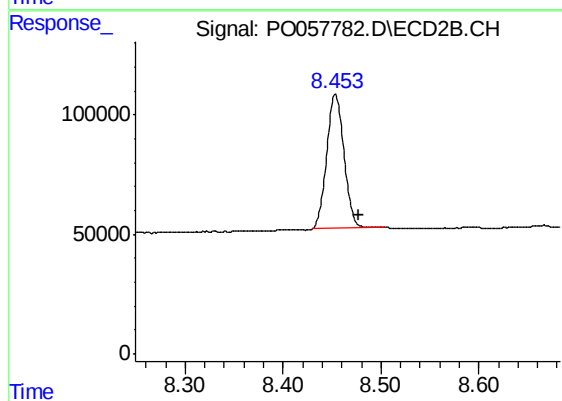

#2 Decachlorobiphenyl

R.T.: 8.453 min
Delta R.T.: -0.023 min
Response: 693466
Conc: 18.54 ng/ml