

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071119\
 Data File : P0057792.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2019 10:56
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 11:25:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.221	3.545	765562	681773	19.489	19.389
2)	SA Decachlor...	9.751	8.457	996193	677476	17.715	18.111
Target Compounds							
20)	L4 AR-1242-5	0.000	5.421	0	38138	N.D.	38.082 #
24)	L5 AR-1248-4	6.226	0.000	96425	0	41.139	N.D. #
25)	L5 AR-1248-5	0.000	5.421	0	38138	N.D.	24.660 #
26)	L6 AR-1254-1	6.226	5.421	96425	38138	49.506	17.933 #
28)	L6 AR-1254-3	6.821	0.000	68923	0	20.847	N.D. #
29)	L6 AR-1254-4	0.000	6.251	0	58130	N.D.	32.294 #
32)	L7 AR-1260-2	0.000	6.251	0	58130	N.D.	21.187 #
45)	L9 AR-1268-5	0.000	8.248	0	200061	N.D.	13.020 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071119\
Data File : P0057792.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2019 10:56
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 11:25:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

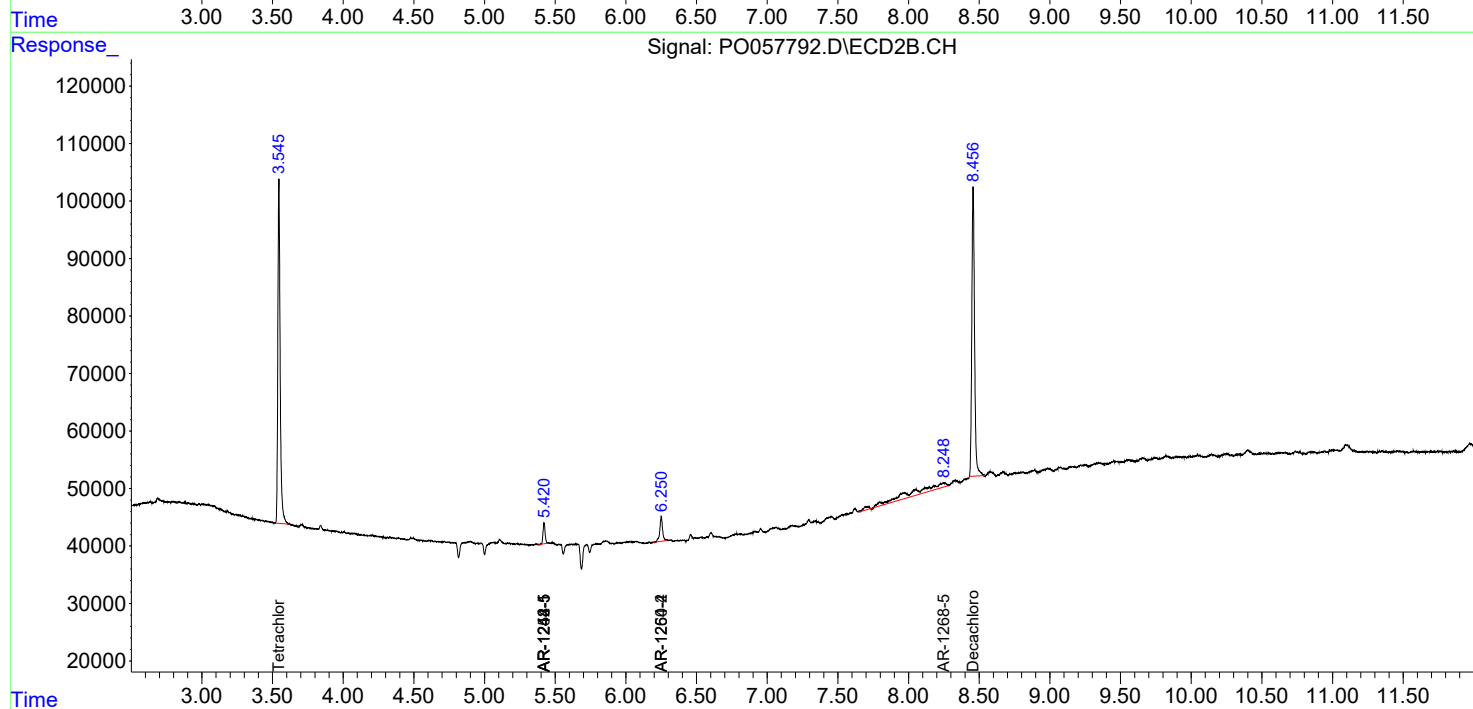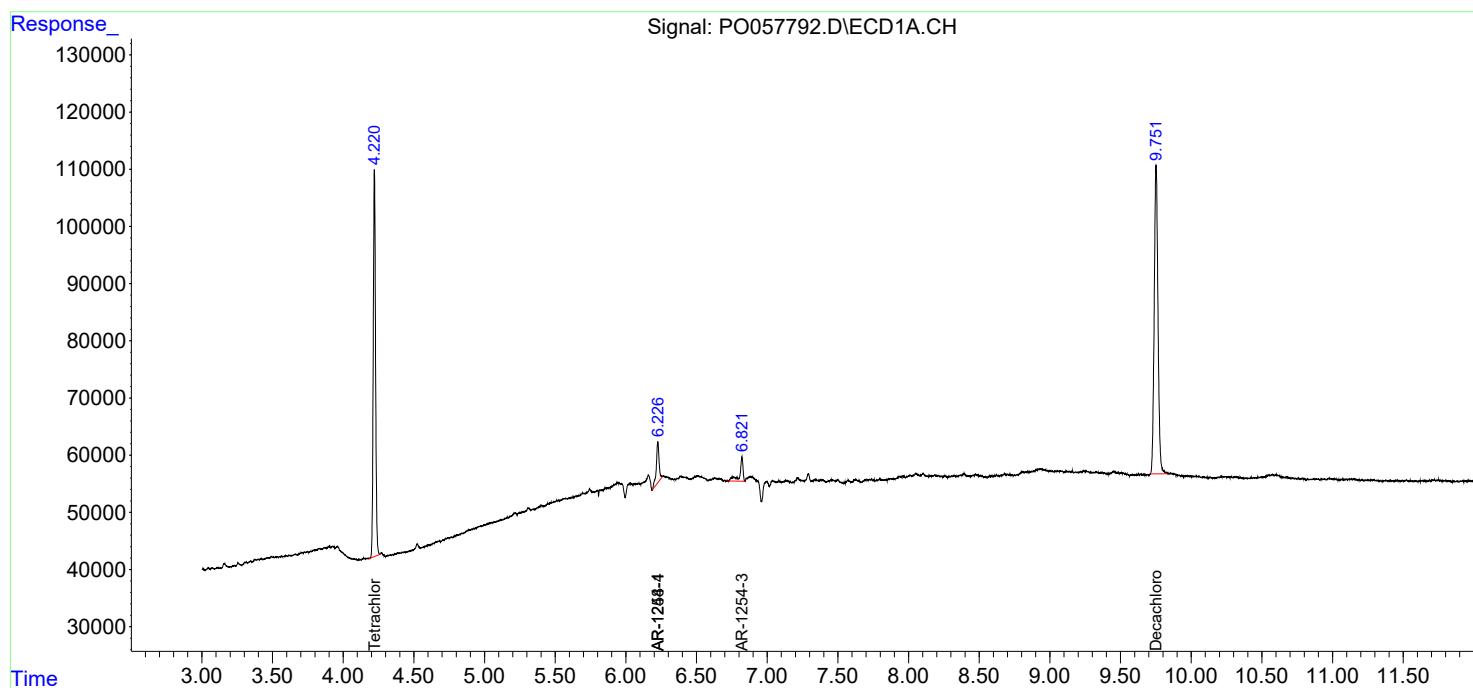


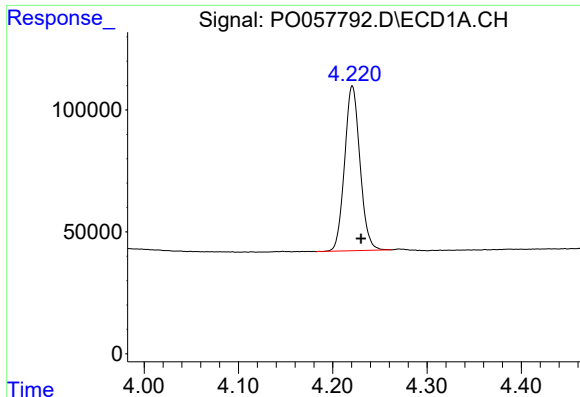

#1 Tetrachloro-m-xylene


R.T.: 4.221 min
Delta R.T.: -0.009 min
Response: 765562
Conc: 19.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

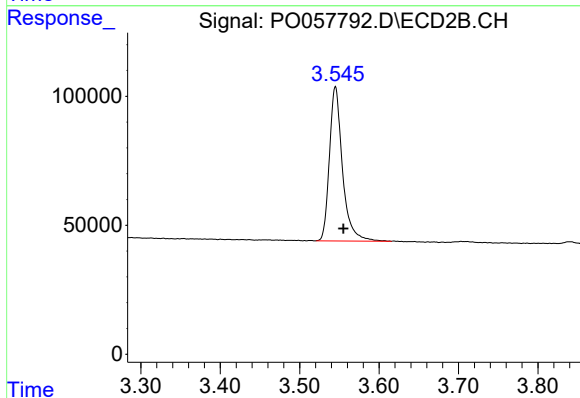


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.010 min
Response: 681773
Conc: 19.39 ng/ml

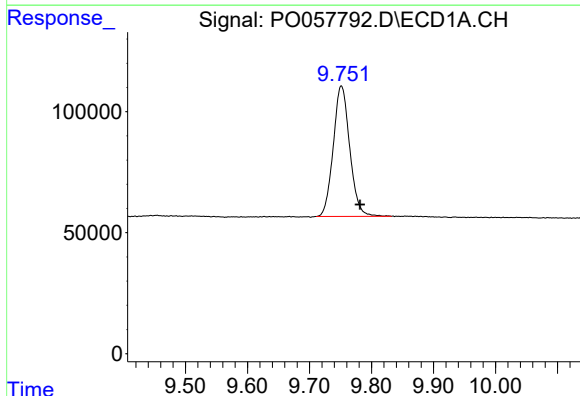


#2 Decachlorobiphenyl

R.T.: 9.751 min
Delta R.T.: -0.030 min
Response: 996193
Conc: 17.72 ng/ml

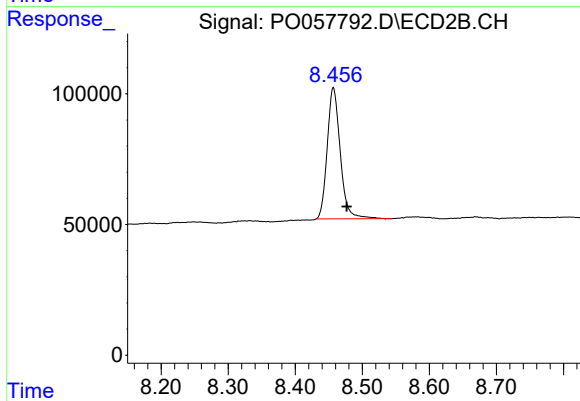

#2 Decachlorobiphenyl


R.T.: 8.457 min
Delta R.T.: -0.020 min
Response: 677476
Conc: 18.11 ng/ml

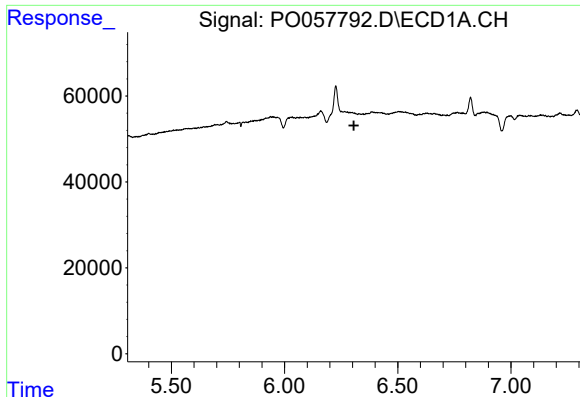

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

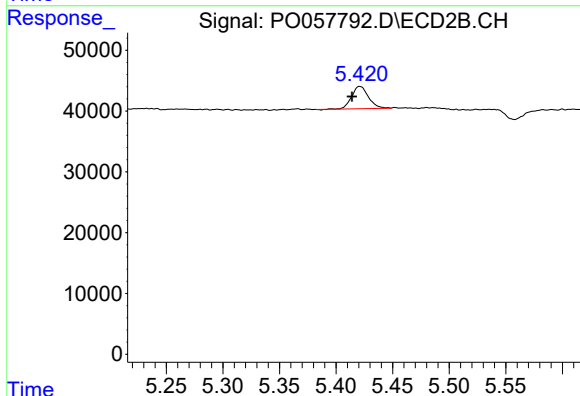


#20 AR-1242-5

R.T.: 5.421 min
Delta R.T.: 0.007 min
Response: 38138
Conc: 38.08 ng/ml

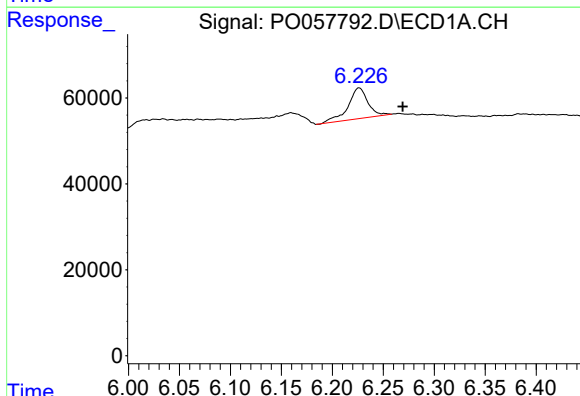


#24 AR-1248-4

R.T.: 6.226 min
Delta R.T.: -0.043 min
Response: 96425
Conc: 41.14 ng/ml

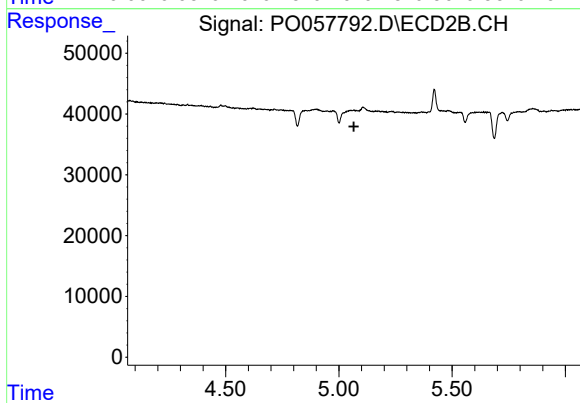

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

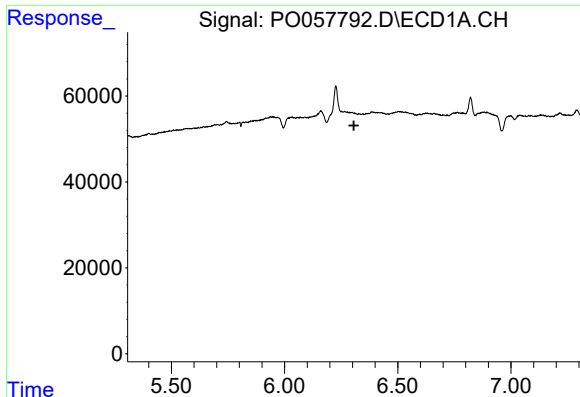

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

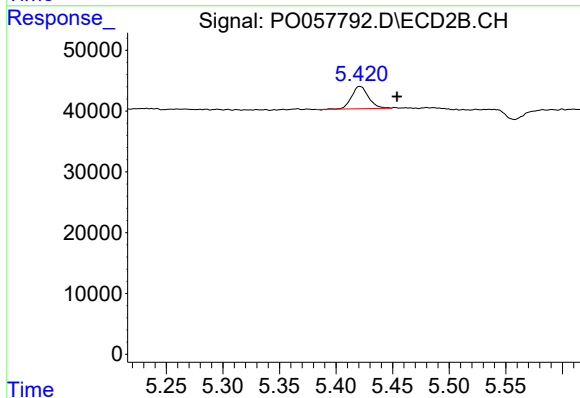


#25 AR-1248-5

R.T.: 5.421 min
Delta R.T.: -0.033 min
Response: 38138
Conc: 24.66 ng/ml

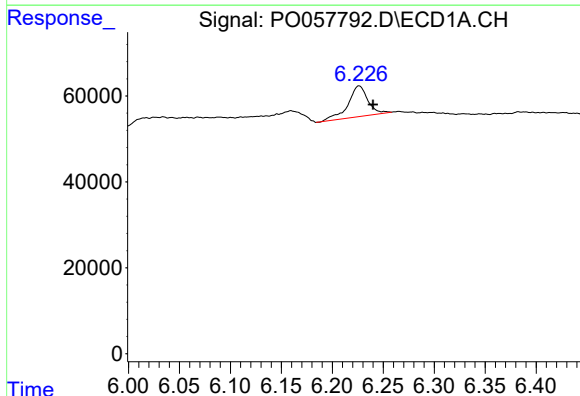


#26 AR-1254-1

R.T.: 6.226 min
Delta R.T.: -0.014 min
Response: 96425
Conc: 49.51 ng/ml

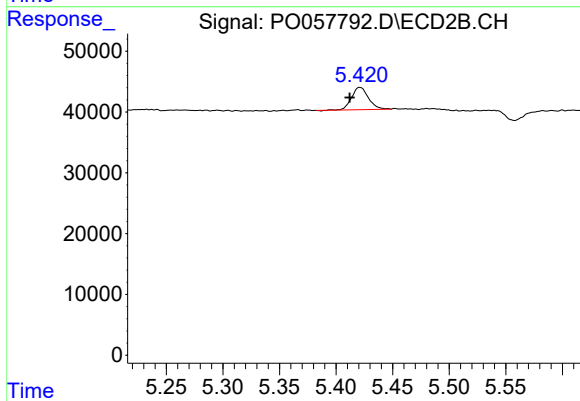

#26 AR-1254-1


R.T.: 5.421 min
Delta R.T.: 0.009 min
Response: 38138
Conc: 17.93 ng/ml

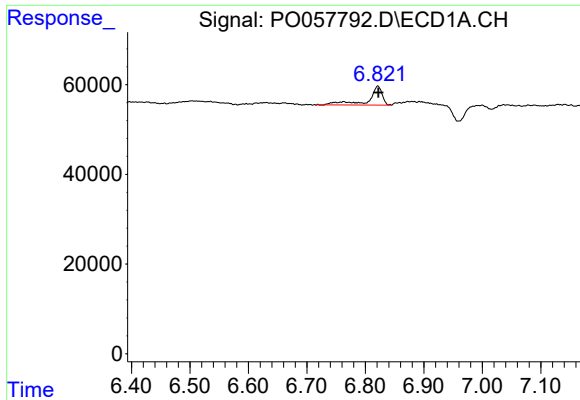

#28 AR-1254-3


R.T.: 6.821 min
Delta R.T.: 0.000 min
Response: 68923
Conc: 20.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

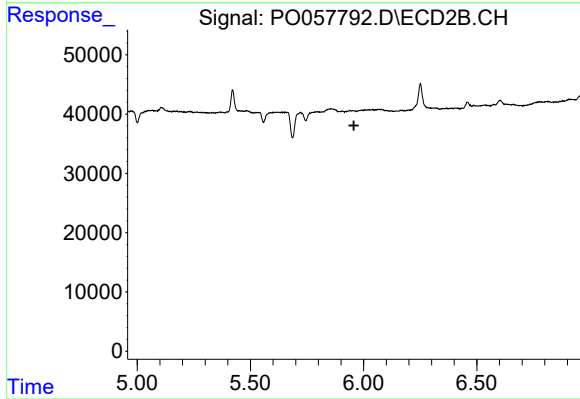


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.957 min
Response: 0
Conc: N.D.

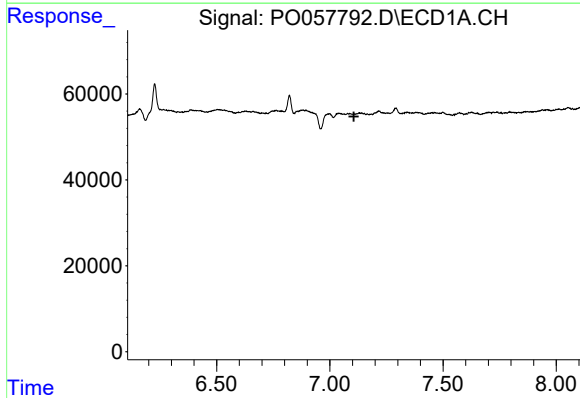


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

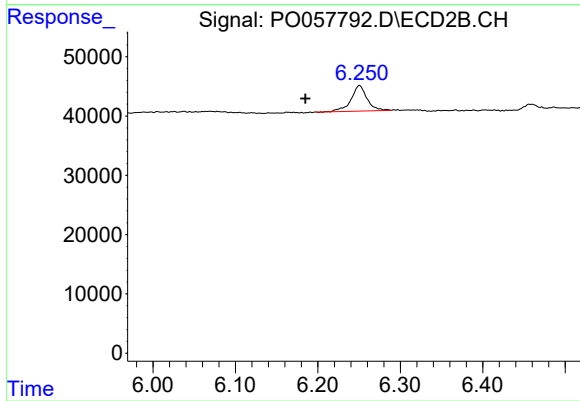

#29 AR-1254-4


R.T.: 6.251 min
Delta R.T.: 0.066 min
Response: 58130
Conc: 32.29 ng/ml

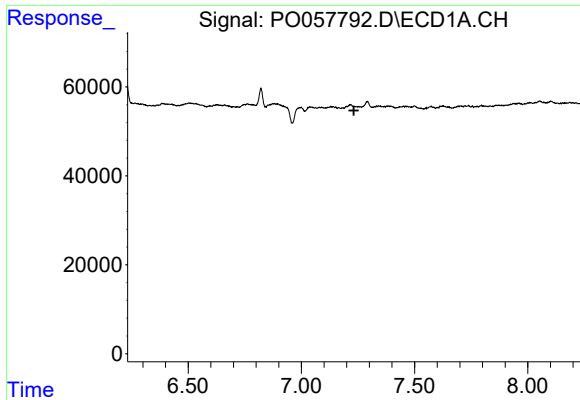

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

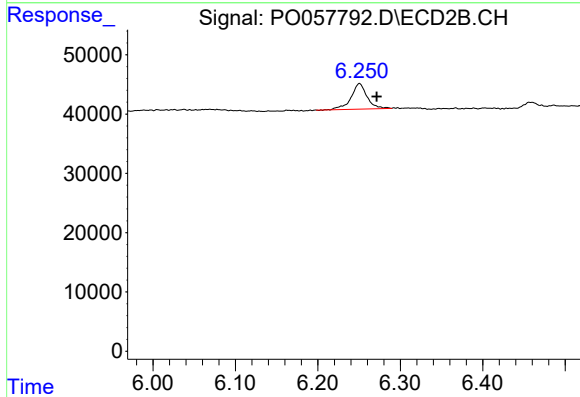


#32 AR-1260-2

R.T.: 6.251 min
Delta R.T.: -0.021 min
Response: 58130
Conc: 21.19 ng/ml

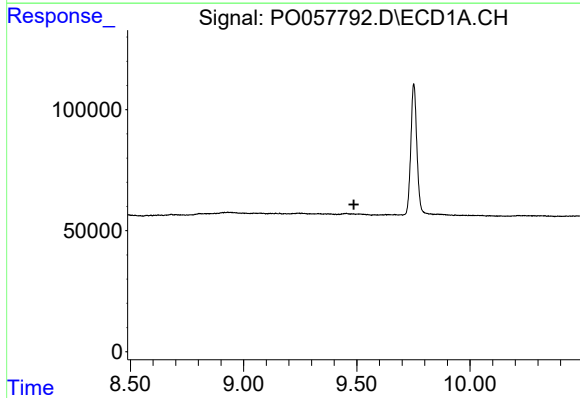

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.487 min
Response: 0
Conc: N.D.

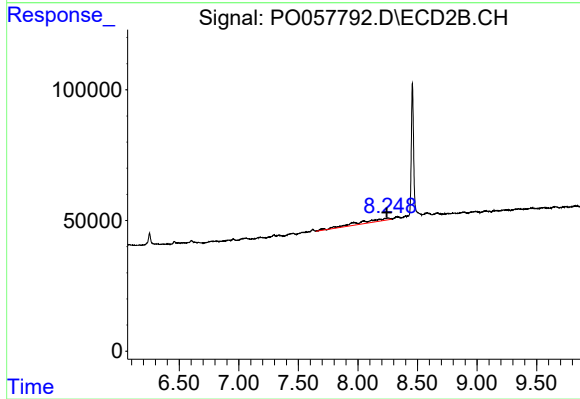

#45 AR-1268-5

R.T.: 8.248 min
Delta R.T.: 0.006 min
Response: 200061
Conc: 13.02 ng/ml