

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071119\
 Data File : P0057797.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2019 13:45
 Operator : SM/SJ
 Sample : K3716-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BLUE-BLOCK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 02:22:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.210	3.545	913745	792445	23.261	22.536
2) SA Decachlor...	9.737	8.458	1170280	1335325	20.811	35.697m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071119\
Data File : PO057797.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2019 13:45
Operator : SM/SJ
Sample : K3716-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BLUE-BLOCK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 02:22:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

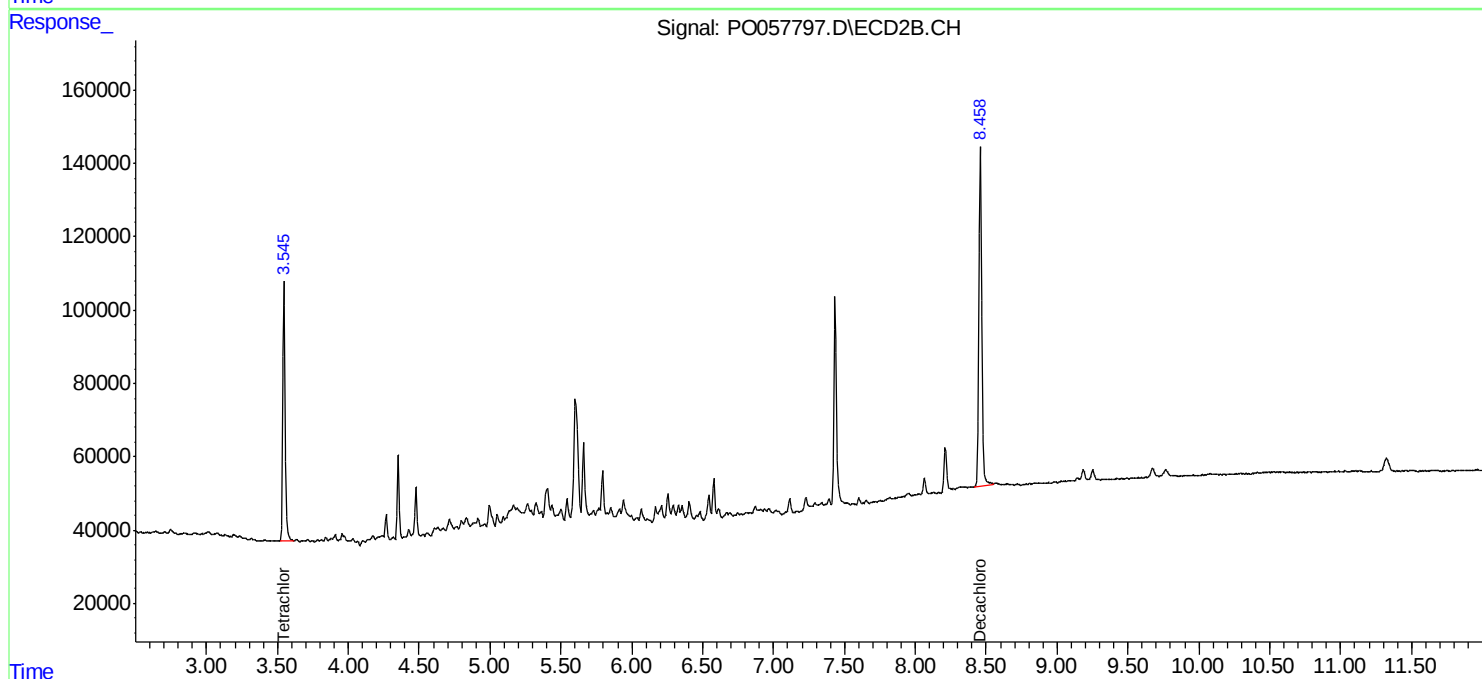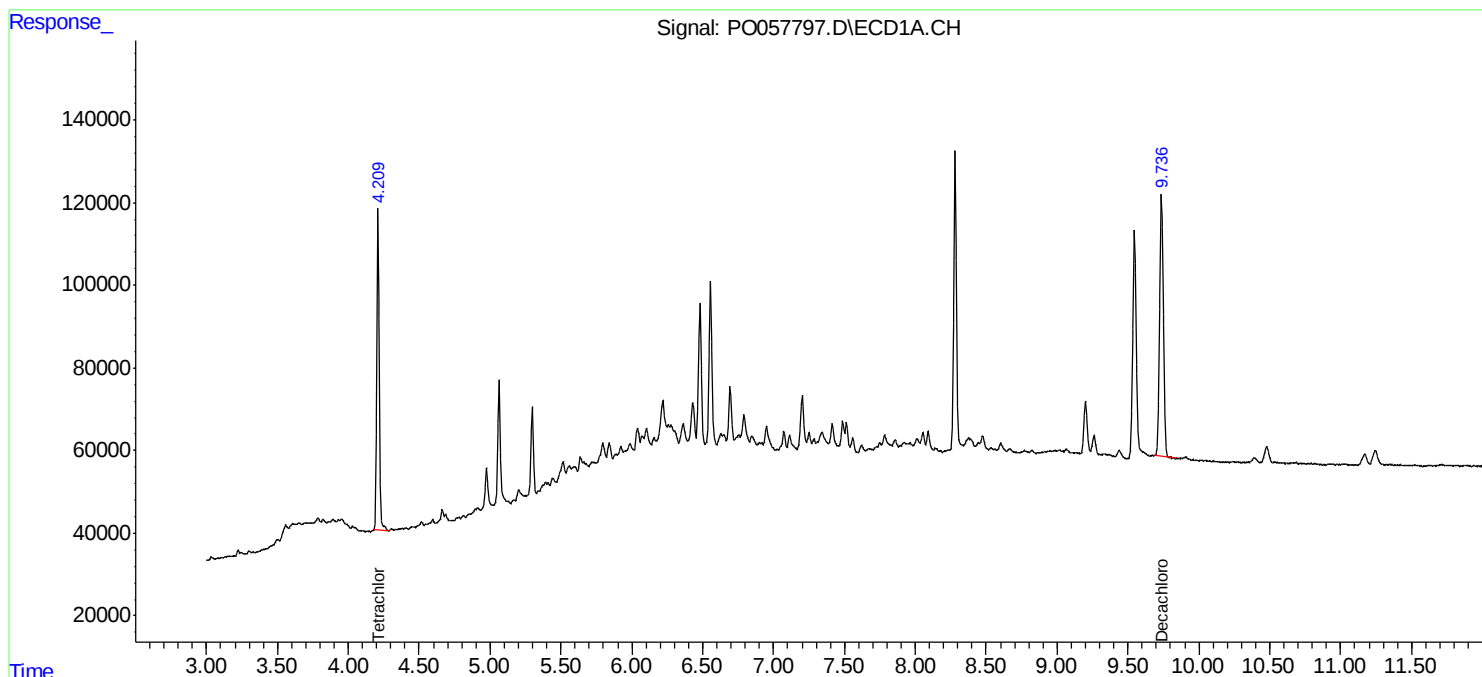


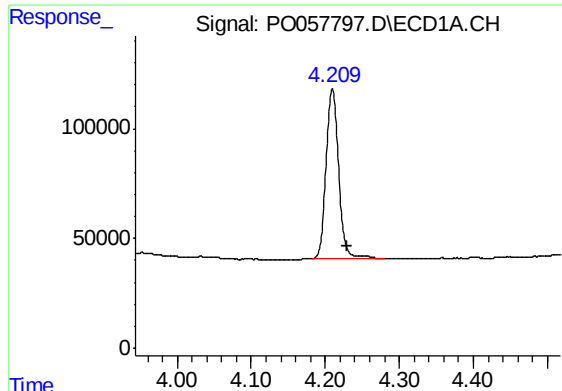

#1 Tetrachloro-m-xylene


R.T.: 4.210 min
Delta R.T.: -0.020 min
Response: 913745
Conc: 23.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
BLUE-BLOCK

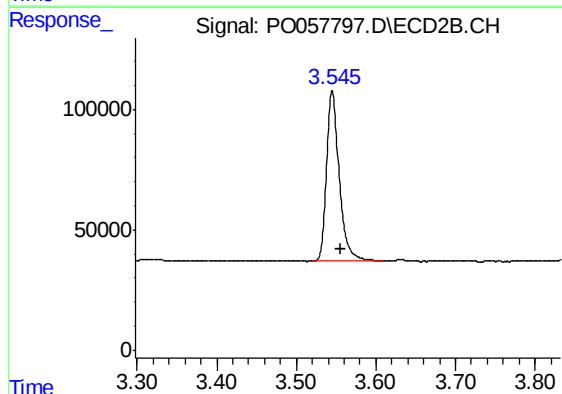


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.010 min
Response: 792445
Conc: 22.54 ng/ml

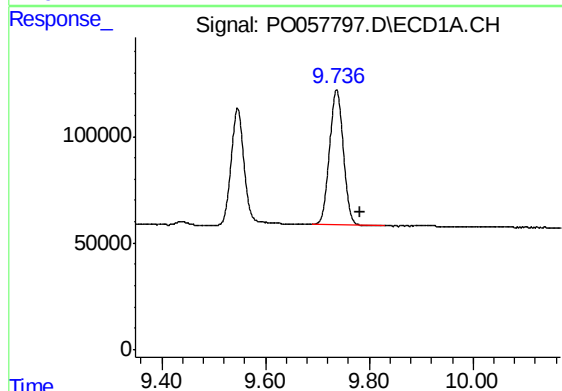

#2 Decachlorobiphenyl

R.T.: 9.737 min
Delta R.T.: -0.044 min
Response: 1170280
Conc: 20.81 ng/ml

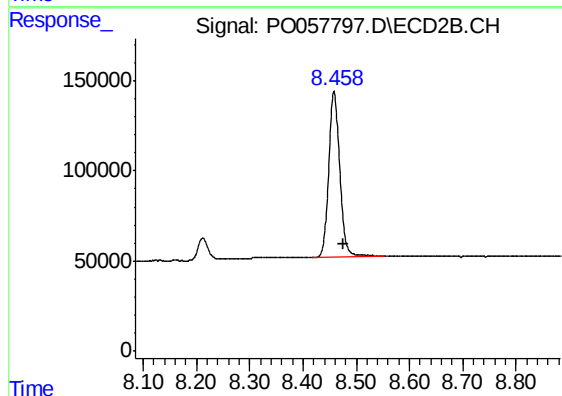

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.019 min
Response: 1335325
Conc: 35.70 ng/ml m