

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071219\
 Data File : P0057851.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jul 2019 21:11
 Operator : SM/SJ
 Sample : K3757-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KY030LC006-SD-190710

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 04:10:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.206	3.543	828445	717060	21.090	20.393
2) SA Decachlor...	9.731	8.452	611064	581060	10.867	15.534 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071219\
Data File : PO057851.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2019 21:11
Operator : SM/SJ
Sample : K3757-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KY030LC006-SD-190710

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:10:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

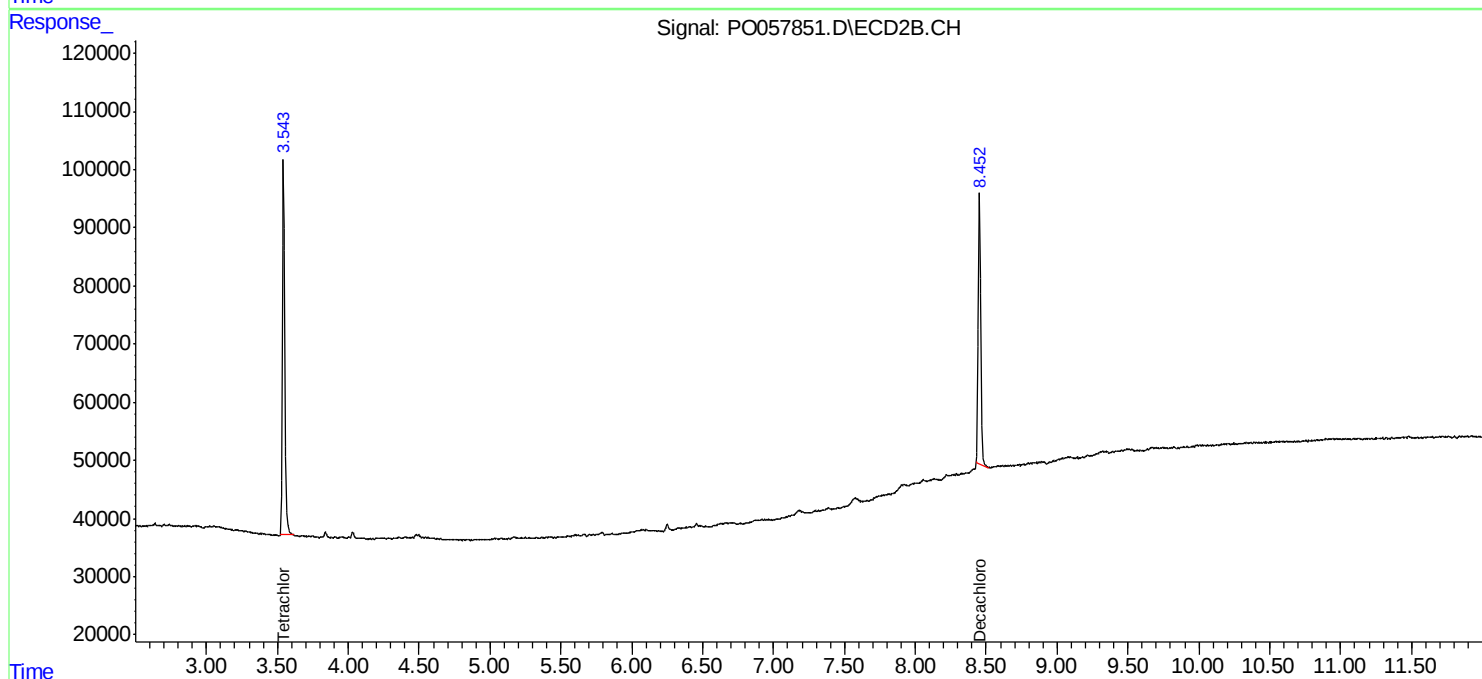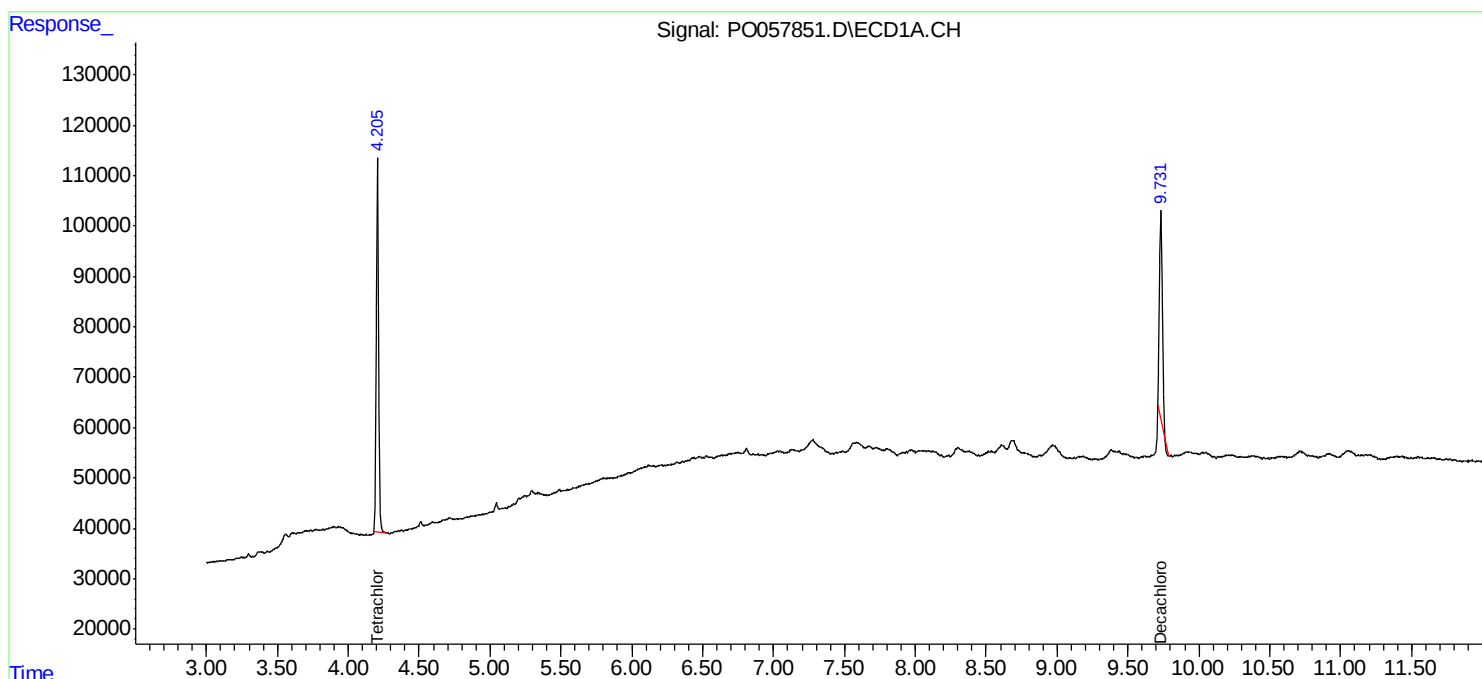


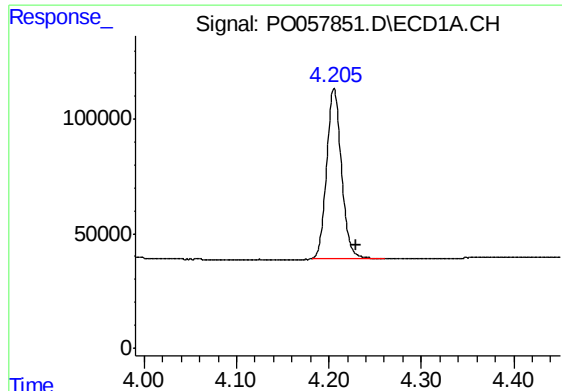

#1 Tetrachloro-m-xylene


R.T.: 4.206 min
Delta R.T.: -0.024 min
Response: 828445
Conc: 21.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
KY030LC006-SD-190710

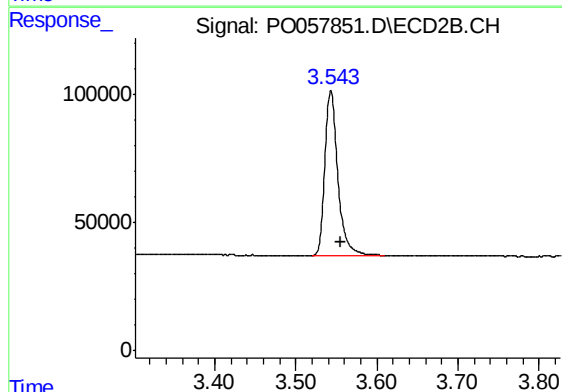


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.012 min
Response: 717060
Conc: 20.39 ng/ml

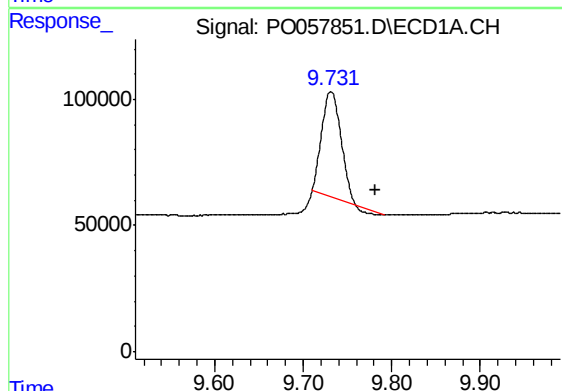

#2 Decachlorobiphenyl

R.T.: 9.731 min
Delta R.T.: -0.050 min
Response: 611064
Conc: 10.87 ng/ml

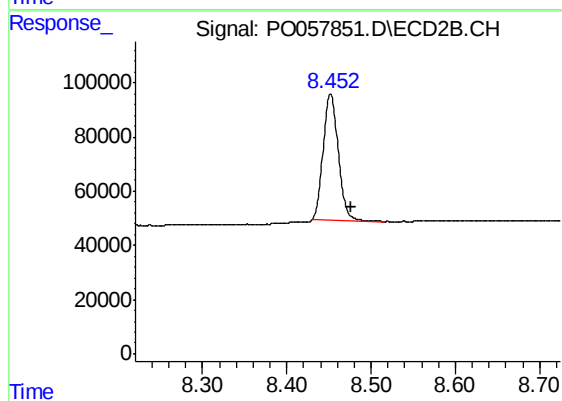

#2 Decachlorobiphenyl

R.T.: 8.452 min
Delta R.T.: -0.025 min
Response: 581060
Conc: 15.53 ng/ml