

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071219\
 Data File : P0057841.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jul 2019 15:40
 Operator : SM/SJ
 Sample : K3739-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K580-B3

Manual Integrations
 APPROVED

Ankita
 7/12/2019 4:28:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 15:55:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.208	3.545	713744	622127	18.170	17.693
2) SA Decachlor...	9.733	8.453	833104	564044	14.815m	15.079m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071219\
Data File : PO057841.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2019 15:40
Operator : SM/SJ
Sample : K3739-03
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K580-B3


Manual Integrations
APPROVED

Ankita
7/12/2019 4:28:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 15:55:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

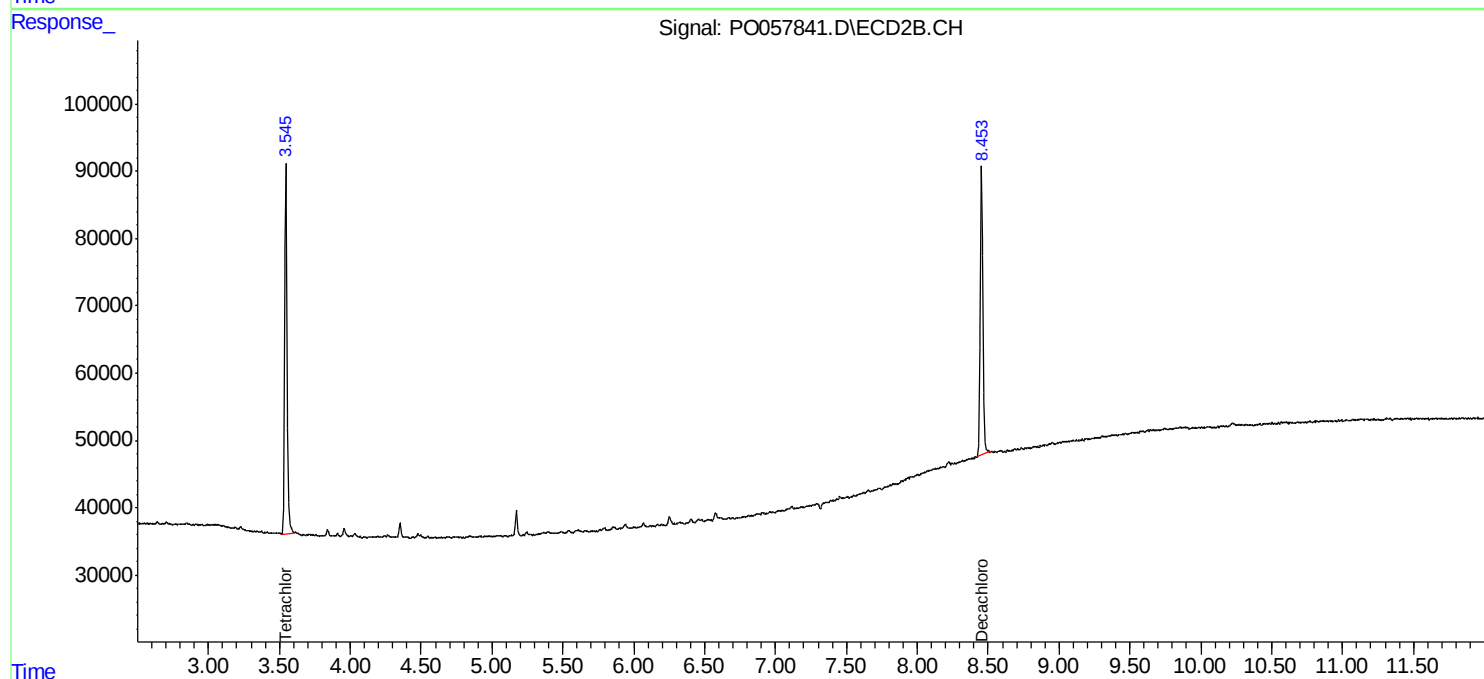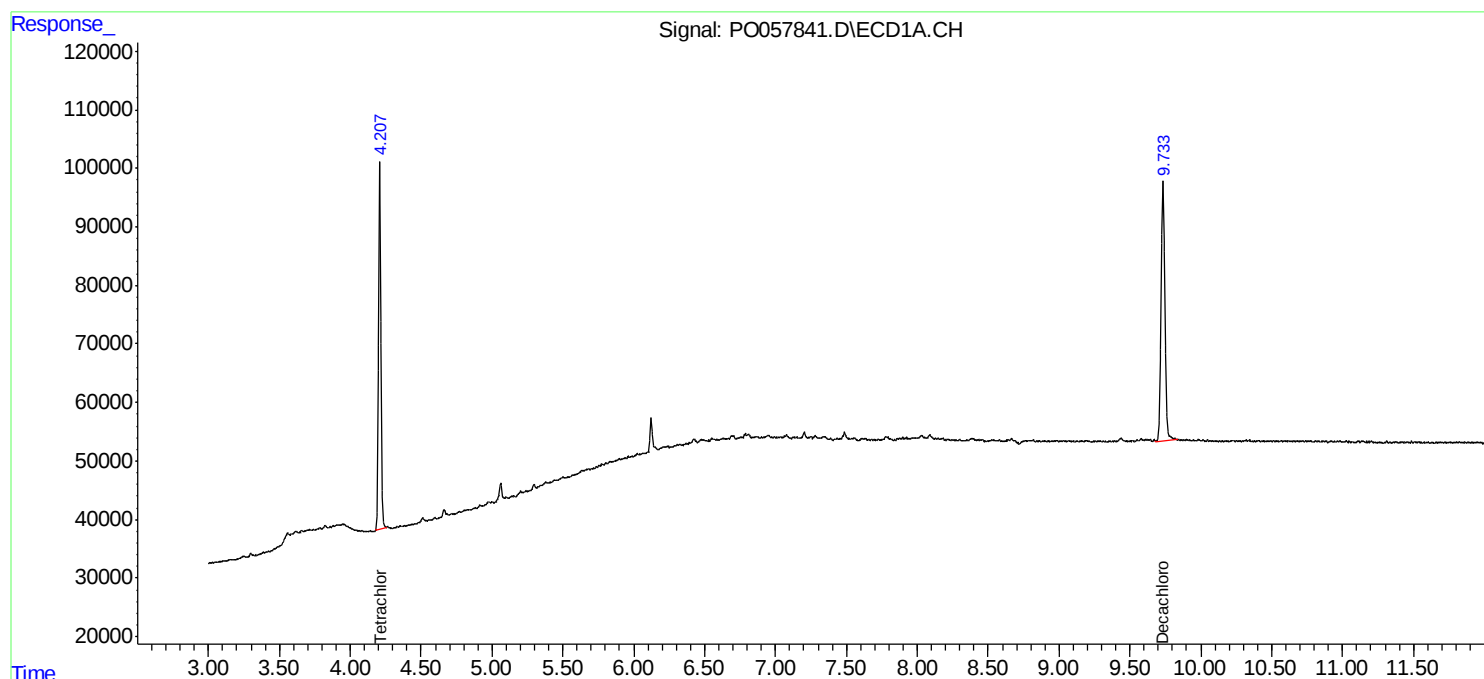

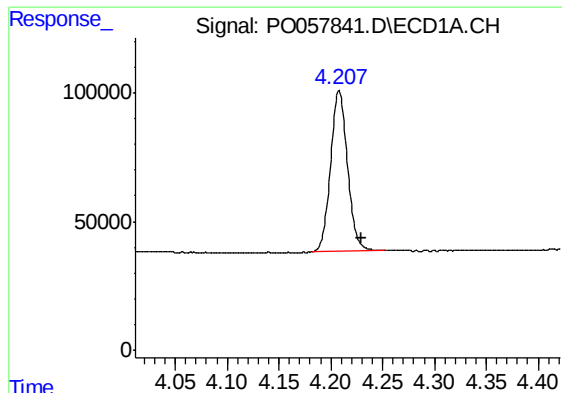


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: -0.022 min
Response: 713744
Conc: 18.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B3


Manual Integrations
APPROVED

Ankita
7/12/2019 4:28:21 PM

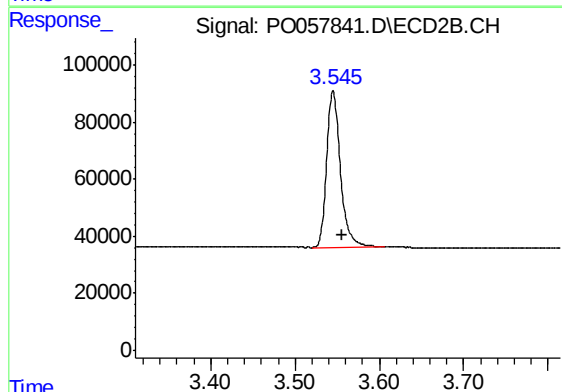


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.010 min
Response: 622127
Conc: 17.69 ng/ml

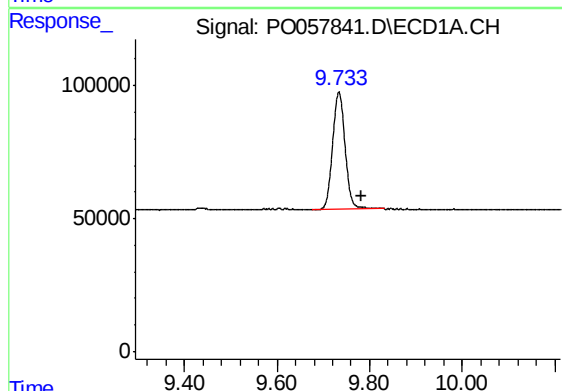

#2 Decachlorobiphenyl

R.T.: 9.733 min
Delta R.T.: -0.048 min
Response: 833104
Conc: 14.82 ng/ml m

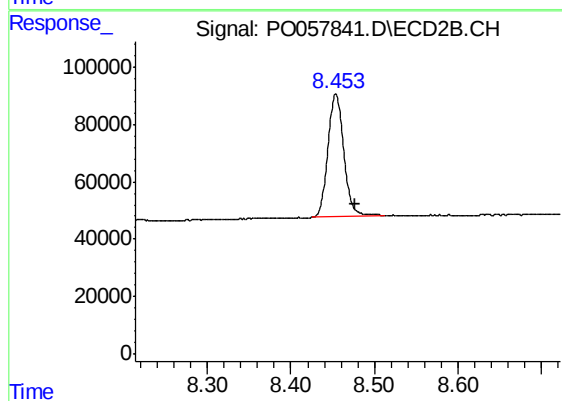

#2 Decachlorobiphenyl

R.T.: 8.453 min
Delta R.T.: -0.024 min
Response: 564044
Conc: 15.08 ng/ml m