

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071319\
 Data File : P0057894.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jul 2019 14:31
 Operator : SM/AJ
 Sample : K3775-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 D-3-ROLL-OFF-DUMPSTER-3

Manual Integrations
 APPROVED

mohammad
 7/15/2019 3:27:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 15:34:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.205	3.544	1172499	971978	29.849m	27.642
2)	SA Decachlor...	9.731	8.452	1169274	807153	20.793m	21.578

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071319\
Data File : PO057894.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2019 14:31
Operator : SM/AJ
Sample : K3775-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
D-3-ROLL-OFF-DUMPSTER-3


Manual Integrations
APPROVED

mohammad
7/15/2019 3:27:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 15:34:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

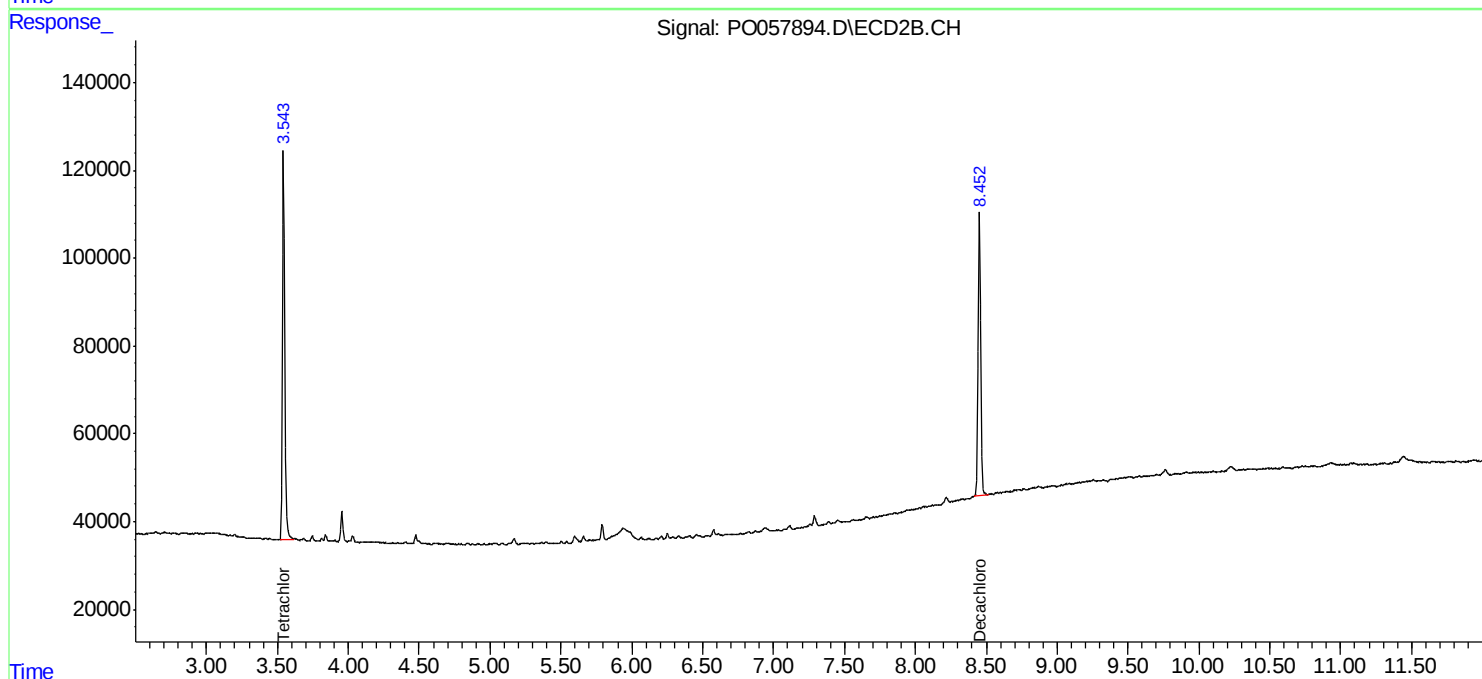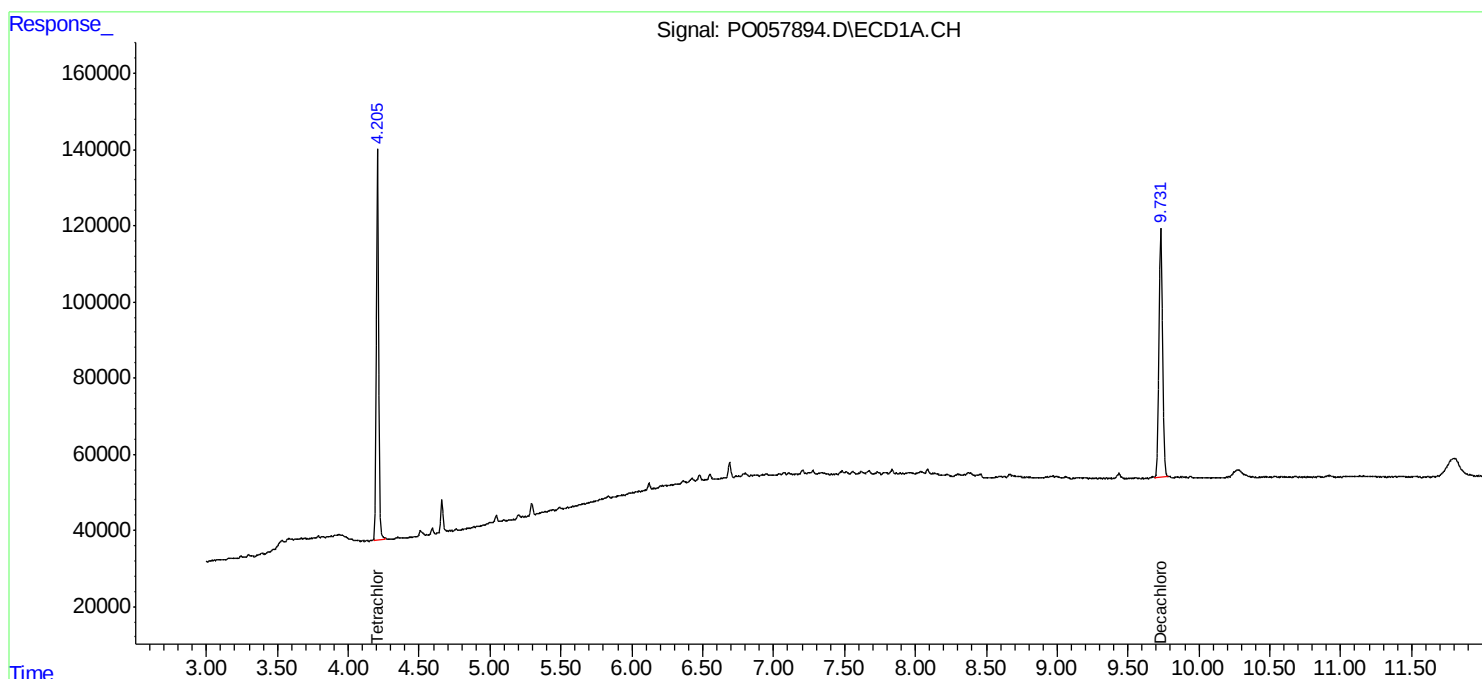

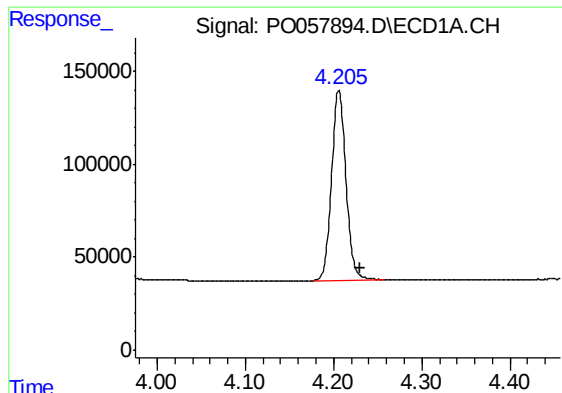


#1 Tetrachloro-m-xylene

R.T.: 4.205 min
Delta R.T.: -0.025 min
Response: 1172499
Conc: 29.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
D-3-ROLL-OFF-DUMPSTER-3


Manual Integrations
APPROVED

mohammad
7/15/2019 3:27:53 PM

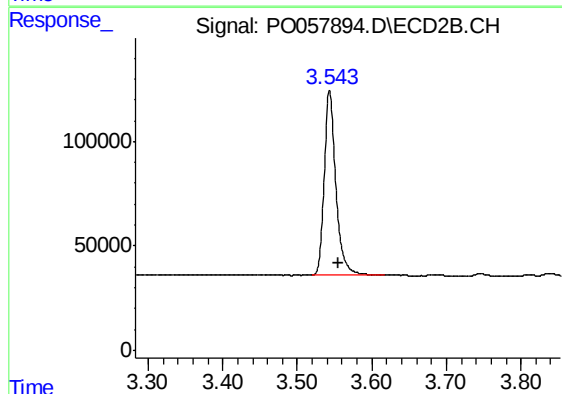


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.012 min
Response: 971978
Conc: 27.64 ng/ml

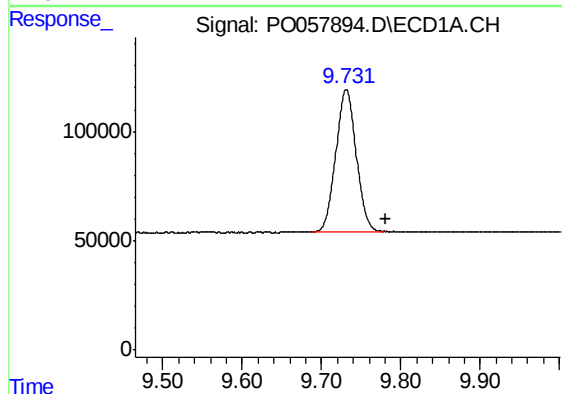

#2 Decachlorobiphenyl

R.T.: 9.731 min
Delta R.T.: -0.050 min
Response: 1169274
Conc: 20.79 ng/ml m

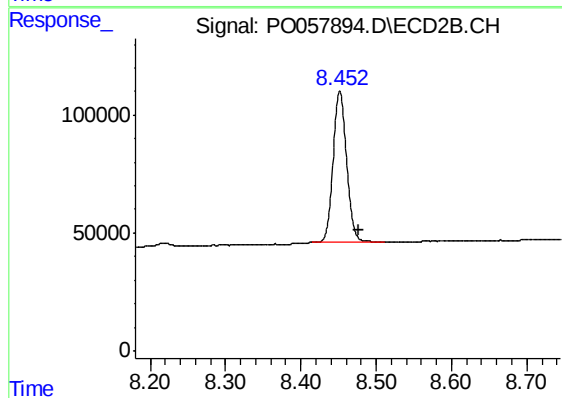

#2 Decachlorobiphenyl

R.T.: 8.452 min
Delta R.T.: -0.025 min
Response: 807153
Conc: 21.58 ng/ml