

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072119\
 Data File : P0058226.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2019 14:12
 Operator : SM/AJ
 Sample : K3914-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S15-3-B

Manual Integrations
 APPROVED

Ankita
 7/22/2019 3:04:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:06:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.196	3.534	776770	730555	22.922	22.777
2)	SA Decachlor...	9.706	8.437	887927	590966	17.356	17.242
Target Compounds							
26)	L6 AR-1254-1	6.192	5.381	14785	16017	7.523m	7.861m
27)	L6 AR-1254-2	6.409	5.528	64692	35607	19.789m	19.649m
28)	L6 AR-1254-3	6.773	5.926	93456	87134	26.491m	29.755
29)	L6 AR-1254-4	7.057	6.153	118485	80639	40.045m	43.644
30)	L6 AR-1254-5	7.471	6.564	197021	182612	67.122m	67.174m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072119\
Data File : PO058226.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2019 14:12
Operator : SM/AJ
Sample : K3914-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S15-3-B


Manual Integrations
APPROVED

Ankita
7/22/2019 3:04:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:06:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

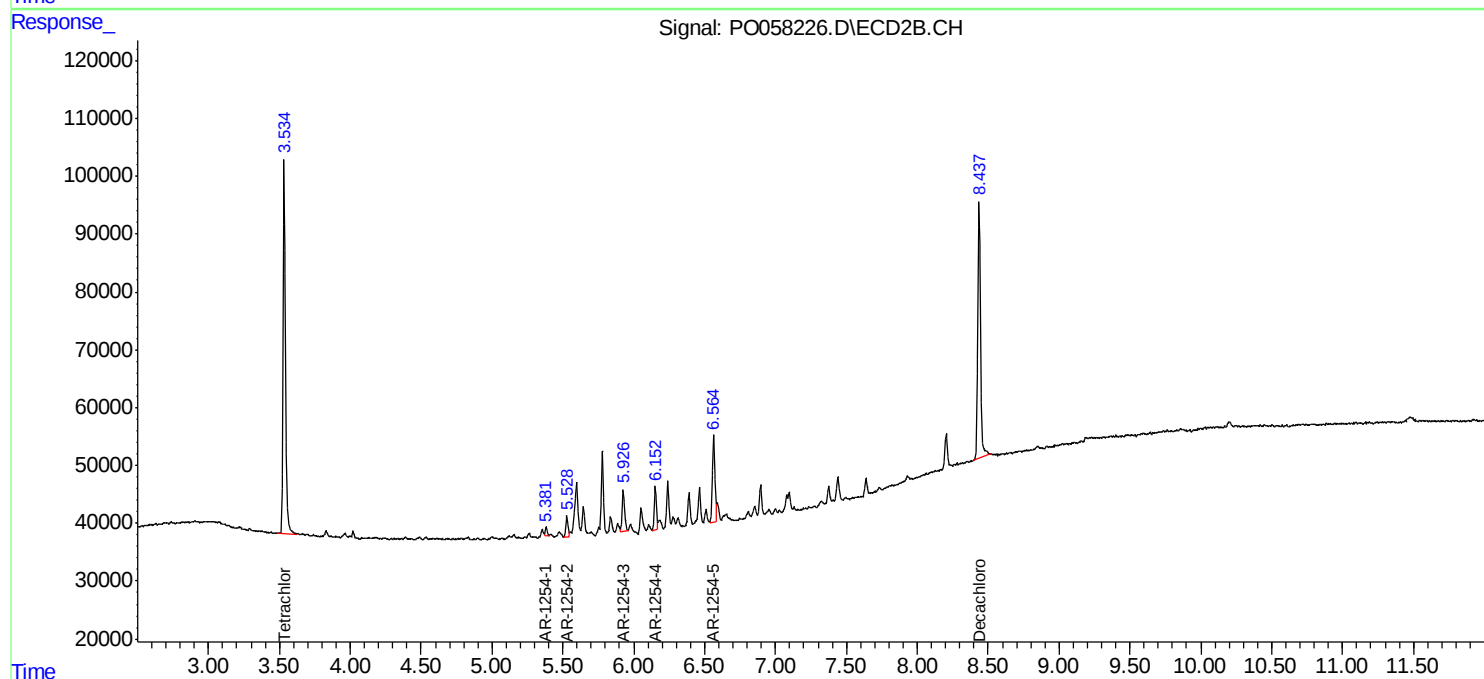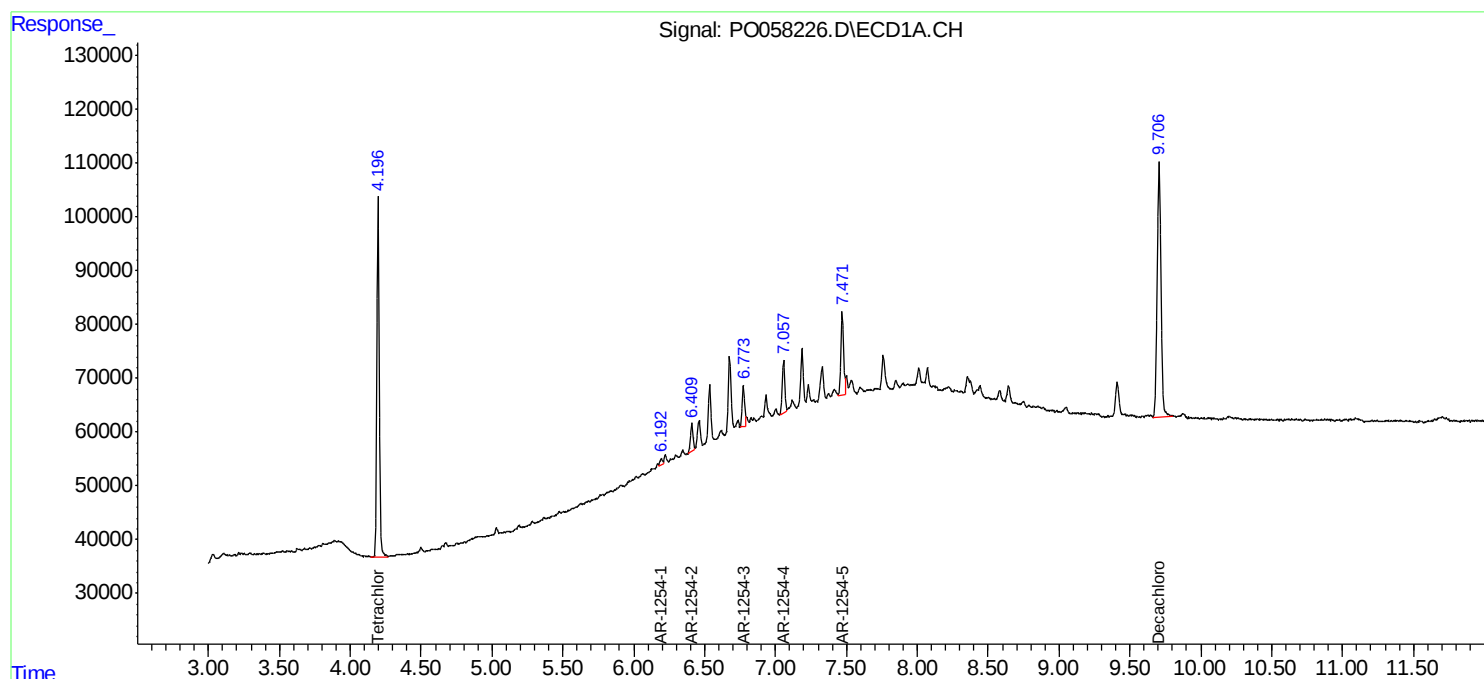

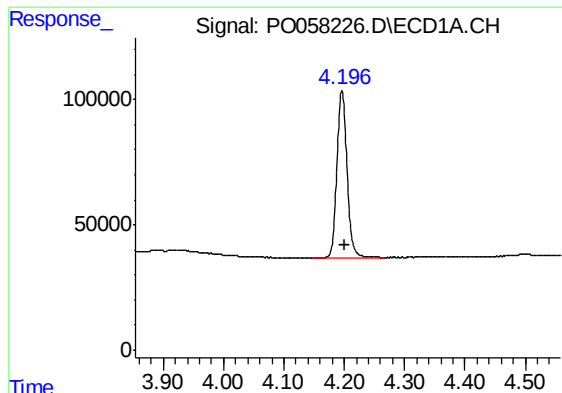


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.004 min
Response: 776770
Conc: 22.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
S15-3-B


Manual Integrations
APPROVED

Ankita
7/22/2019 3:04:12 PM

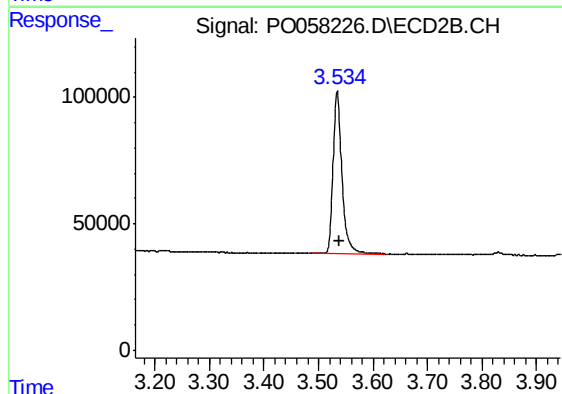


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.005 min
Response: 730555
Conc: 22.78 ng/ml

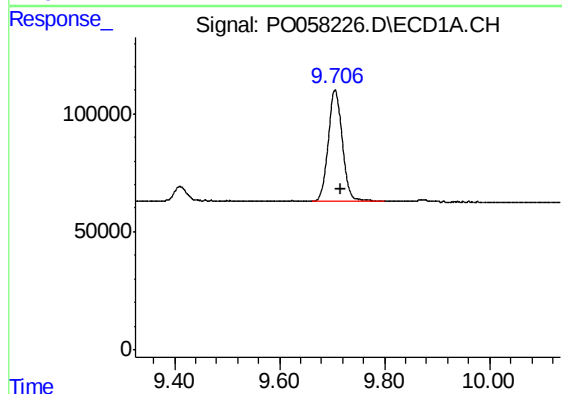


#2 Decachlorobiphenyl

R.T.: 9.706 min
Delta R.T.: -0.012 min
Response: 887927
Conc: 17.36 ng/ml

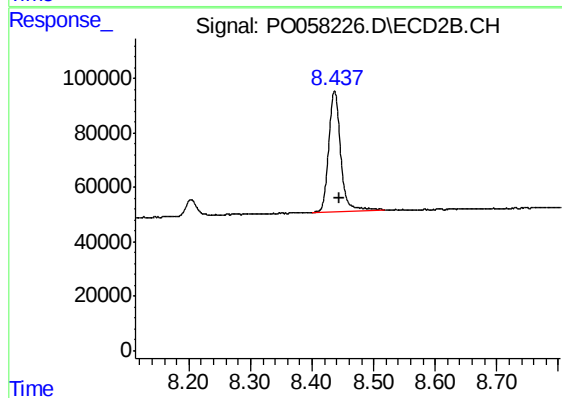

#2 Decachlorobiphenyl

R.T.: 8.437 min
Delta R.T.: -0.008 min
Response: 590966
Conc: 17.24 ng/ml

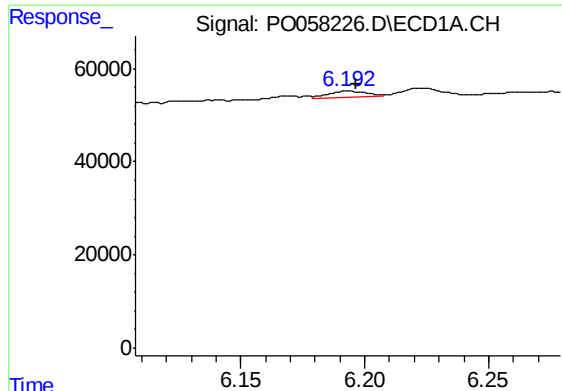


#26 AR-1254-1

R.T.: 6.192 min
Delta R.T.: -0.004 min
Response: 14785
Conc: 7.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S15-3-B


Manual Integrations
APPROVED

Ankita
7/22/2019 3:04:12 PM

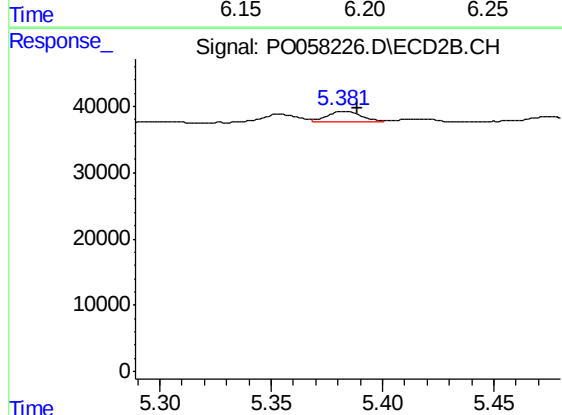


#26 AR-1254-1

R.T.: 5.381 min
Delta R.T.: -0.008 min
Response: 16017
Conc: 7.86 ng/ml m

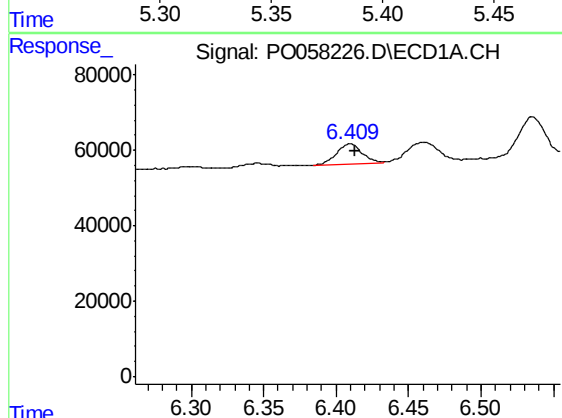


#27 AR-1254-2

R.T.: 6.409 min
Delta R.T.: -0.003 min
Response: 64692
Conc: 19.79 ng/ml m

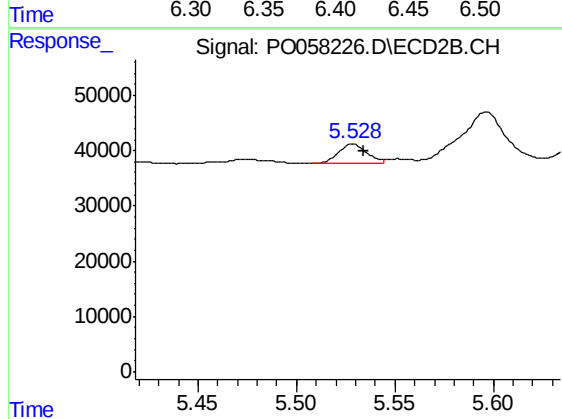

#27 AR-1254-2

R.T.: 5.528 min
Delta R.T.: -0.006 min
Response: 35607
Conc: 19.65 ng/ml m

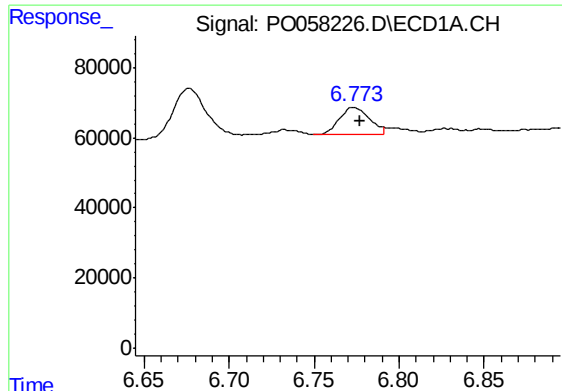


#28 AR-1254-3

R.T.: 6.773 min
Delta R.T.: -0.004 min
Response: 93456
Conc: 26.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S15-3-B


Manual Integrations
APPROVED

Ankita
7/22/2019 3:04:12 PM

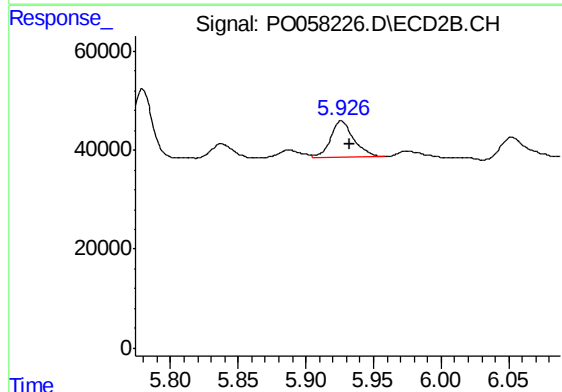


#28 AR-1254-3

R.T.: 5.926 min
Delta R.T.: -0.006 min
Response: 87134
Conc: 29.75 ng/ml

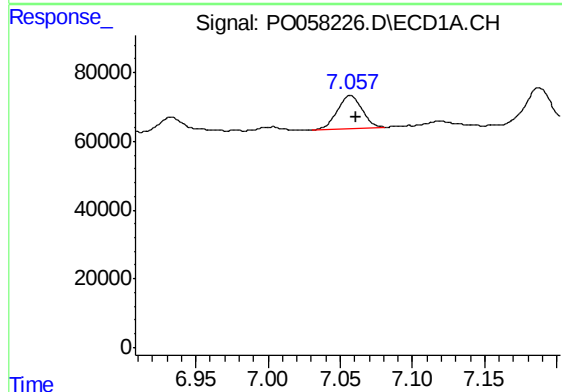


#29 AR-1254-4

R.T.: 7.057 min
Delta R.T.: -0.005 min
Response: 118485
Conc: 40.04 ng/ml m

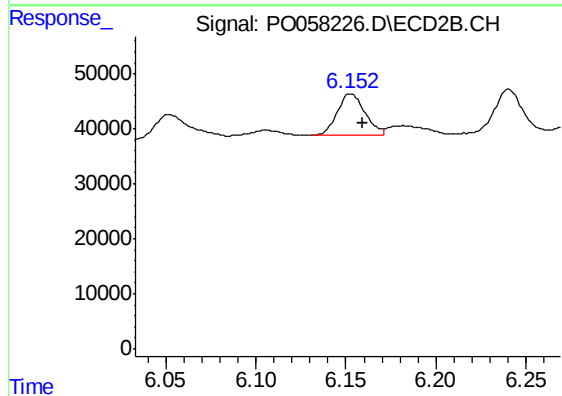

#29 AR-1254-4

R.T.: 6.153 min
Delta R.T.: -0.006 min
Response: 80639
Conc: 43.64 ng/ml

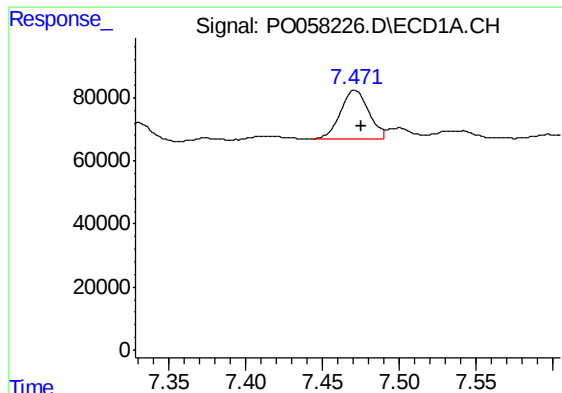


#30 AR-1254-5

R.T.: 7.471 min
Delta R.T.: -0.005 min
Response: 197021
Conc: 67.12 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S15-3-B

Manual Integrations
APPROVED

Ankita
7/22/2019 3:04:12 PM

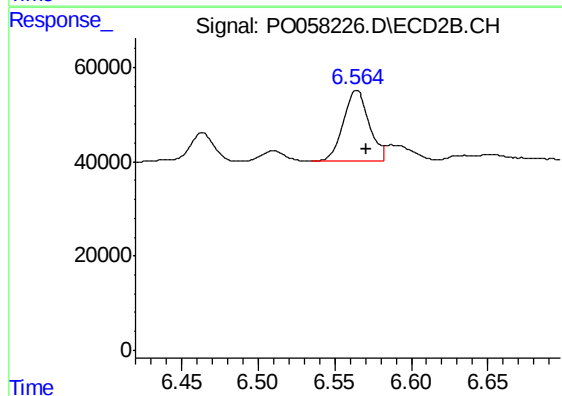

#30 AR-1254-5

R.T.: 6.564 min
Delta R.T.: -0.007 min
Response: 182612
Conc: 67.17 ng/ml m