

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
Data File : P0058250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2019 10:08
Operator : SM/AJ
Sample : K3918-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S3-01-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 10:31:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.187	3.532	866388	831385	25.567	25.921
2) SA Decachlor...	9.692	8.431	895880	577247	17.512	16.841

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
Data File : P0058250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2019 10:08
Operator : SM/AJ
Sample : K3918-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S3-01-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 10:31:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

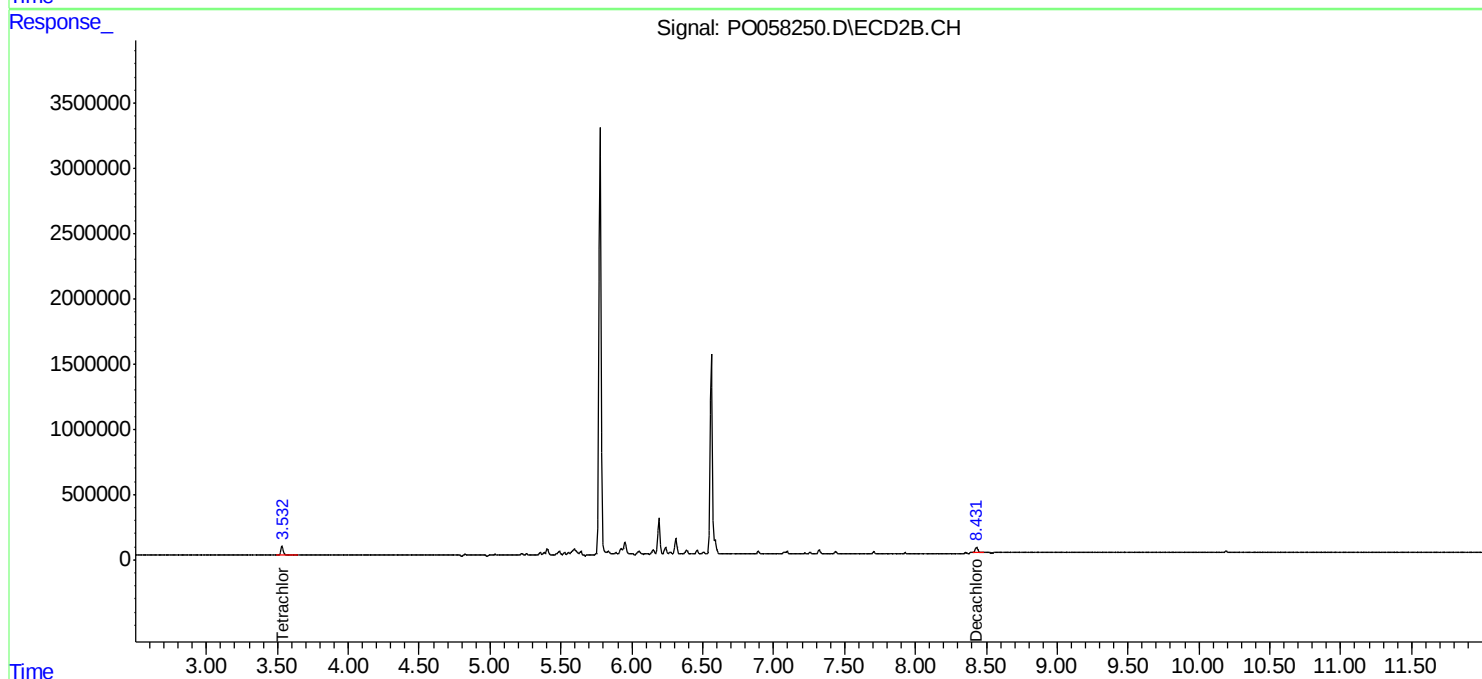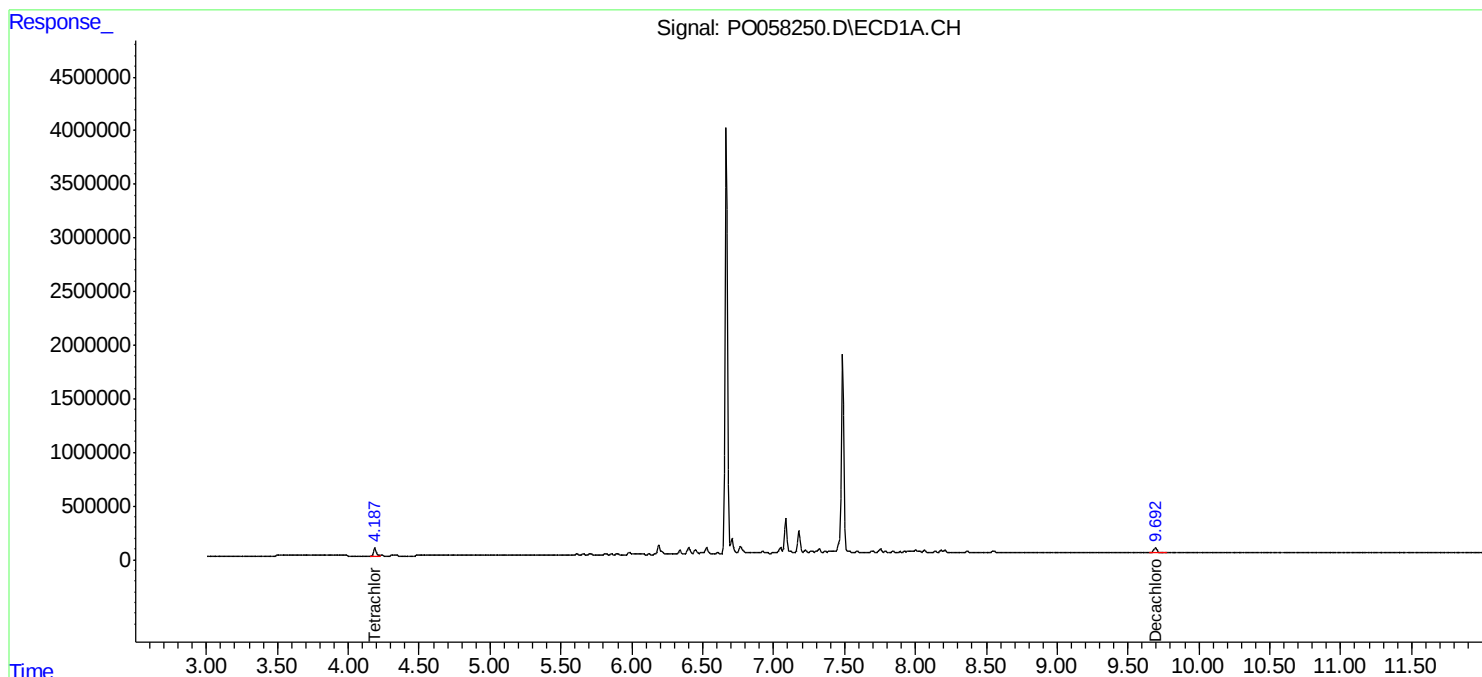


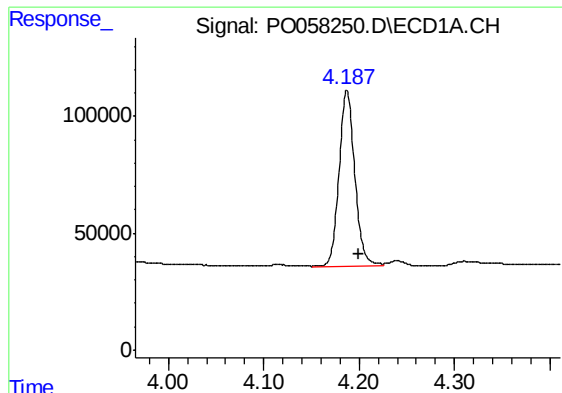

#1 Tetrachloro-m-xylene


R.T.: 4.187 min
Delta R.T.: -0.013 min
Response: 866388
Conc: 25.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-01-S

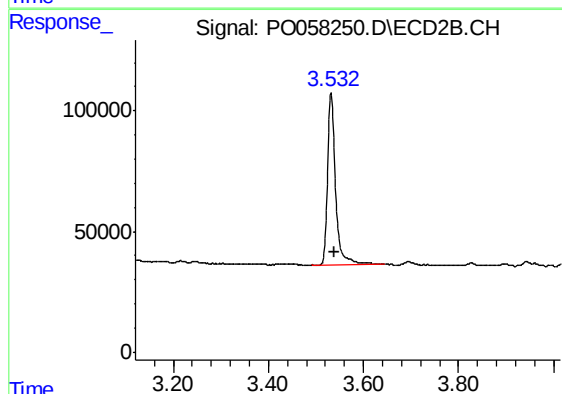


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.007 min
Response: 831385
Conc: 25.92 ng/ml

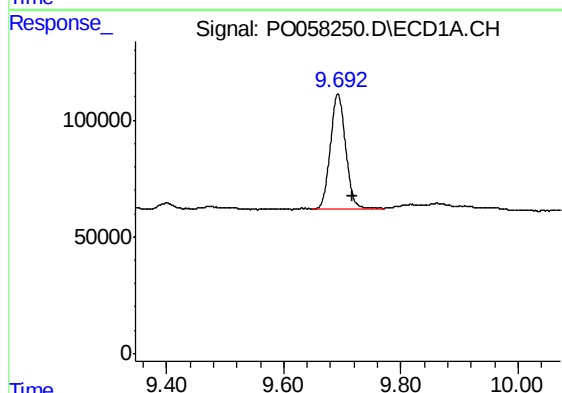

#2 Decachlorobiphenyl

R.T.: 9.692 min
Delta R.T.: -0.026 min
Response: 895880
Conc: 17.51 ng/ml

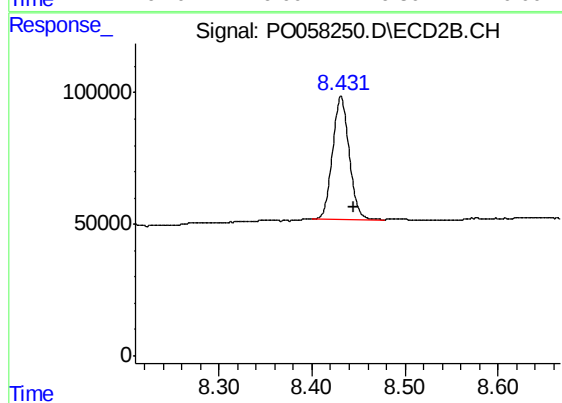

#2 Decachlorobiphenyl

R.T.: 8.431 min
Delta R.T.: -0.014 min
Response: 577247
Conc: 16.84 ng/ml