

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
 Data File : P0058268.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2019 16:46
 Operator : SM/AJ
 Sample : K3858-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-EW03-TRENCHRE

Manual Integrations
 APPROVED

Ankita
 7/23/2019 2:23:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 17:01:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.187	3.534	883368	779915	26.068	24.316
2) SA Decachlor...	9.692	8.432	1334484	890827	26.085m	25.990

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
Data File : P0058268.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2019 16:46
Operator : SM/AJ
Sample : K3858-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IDW-EW03-TRENCHRE


Manual Integrations
APPROVED

Ankita
7/23/2019 2:23:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 17:01:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

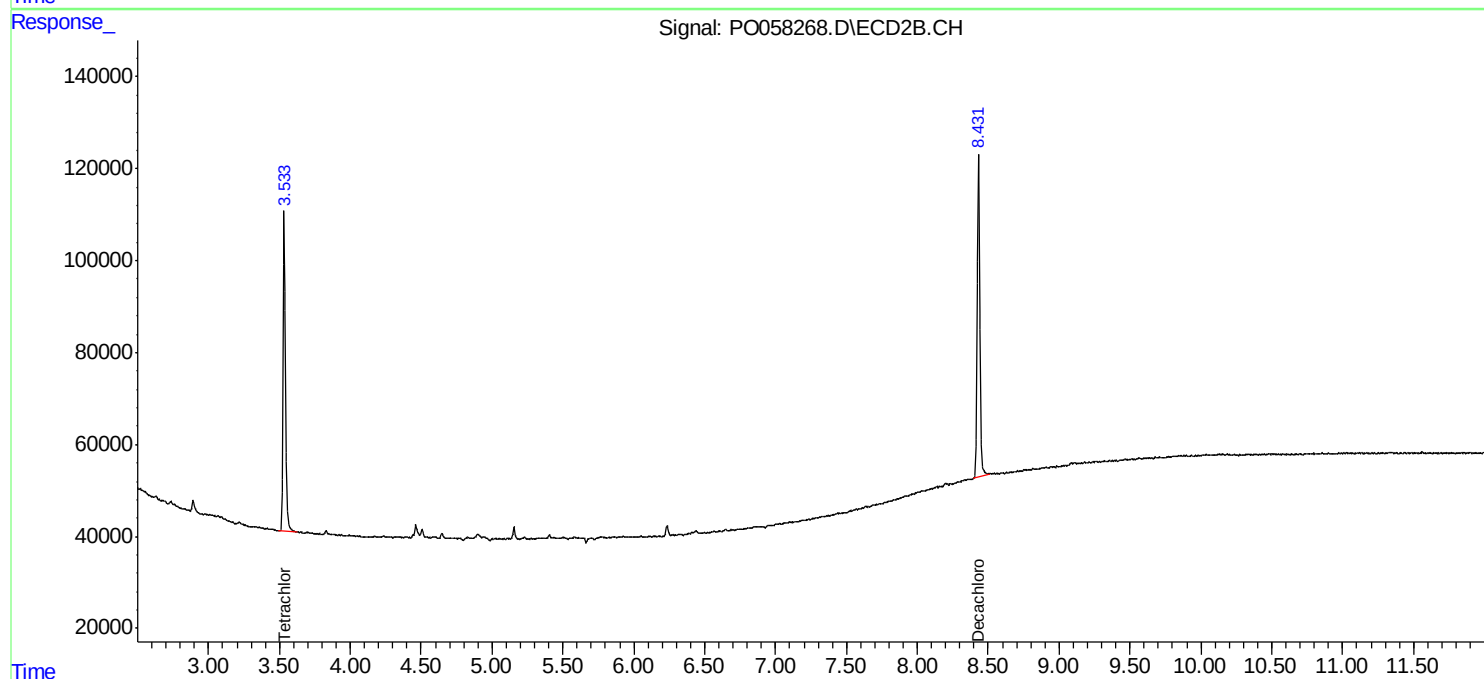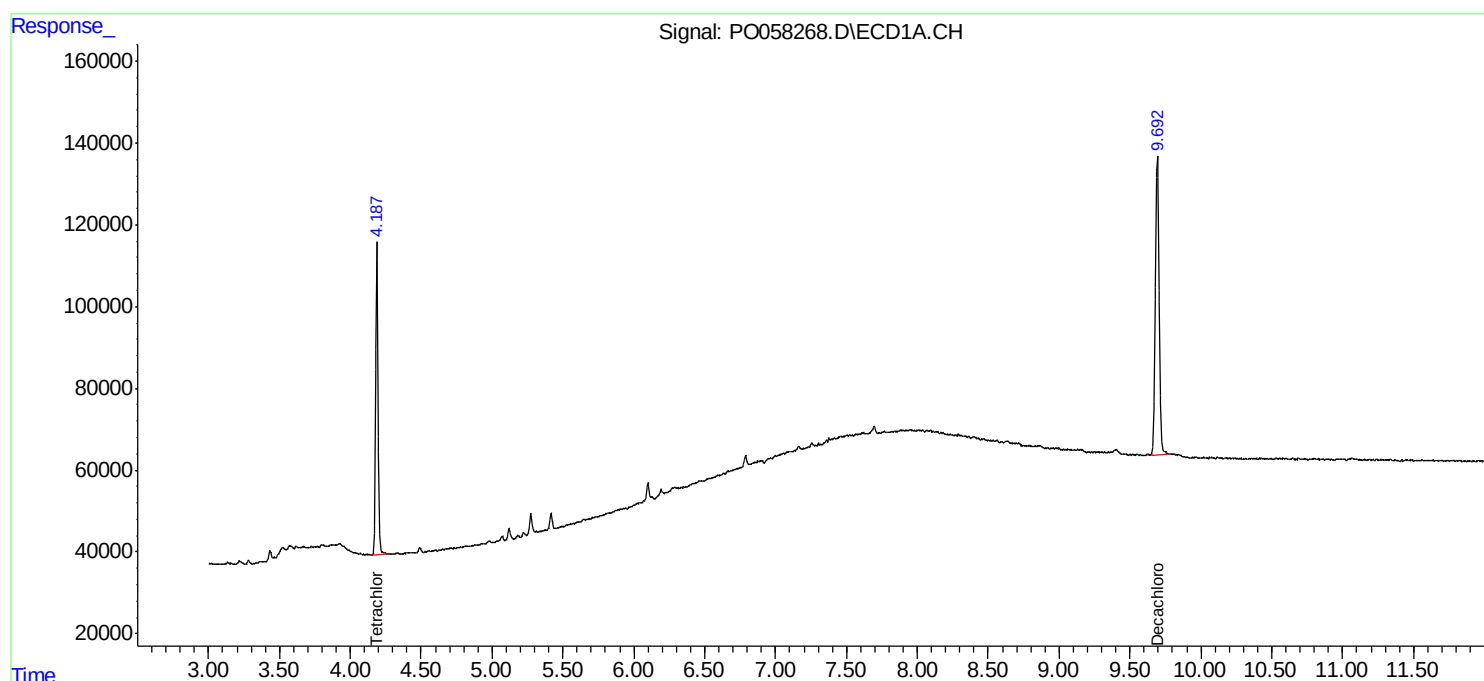

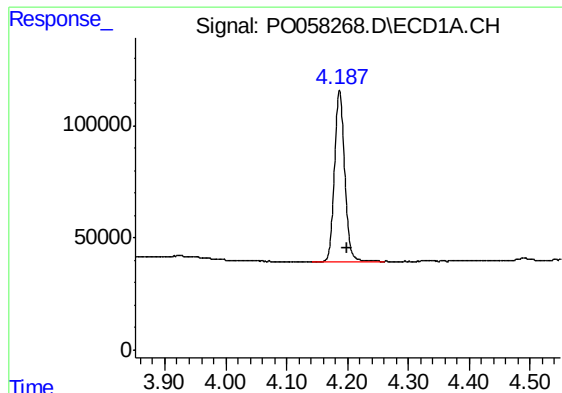


#1 Tetrachloro-m-xylene

R.T.: 4.187 min
Delta R.T.: -0.013 min
Response: 883368
Conc: 26.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-EW03-TRENCHRE


Manual Integrations
APPROVED

Ankita
7/23/2019 2:23:50 PM

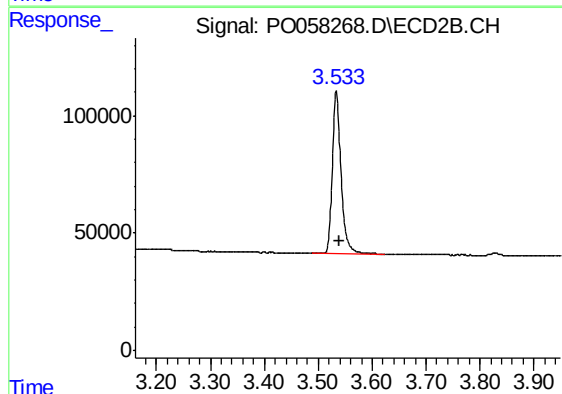


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.006 min
Response: 779915
Conc: 24.32 ng/ml

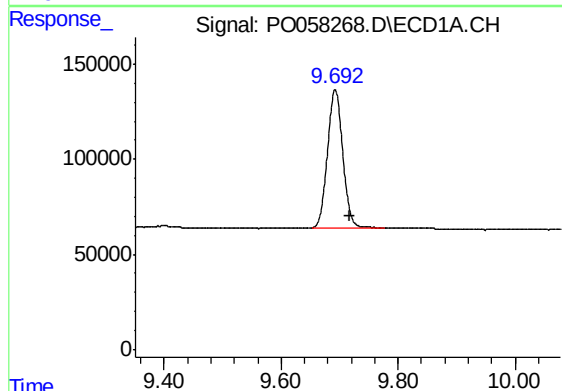

#2 Decachlorobiphenyl

R.T.: 9.692 min
Delta R.T.: -0.026 min
Response: 1334484
Conc: 26.08 ng/ml m

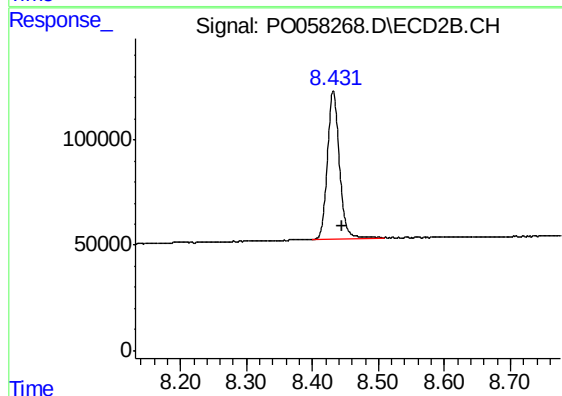

#2 Decachlorobiphenyl

R.T.: 8.432 min
Delta R.T.: -0.014 min
Response: 890827
Conc: 25.99 ng/ml