

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
 Data File : P0058269.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2019 17:03
 Operator : SM/AJ
 Sample : K3858-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-EW03-CONCRETE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 17:19:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.187	3.534	766671	679414	22.624	21.183
2)	SA Decachlor...	9.693	8.432	1340396	886183	26.200	25.855

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
Data File : P0058269.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2019 17:03
Operator : SM/AJ
Sample : K3858-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDW-EW03-CONCRETE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 17:19:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

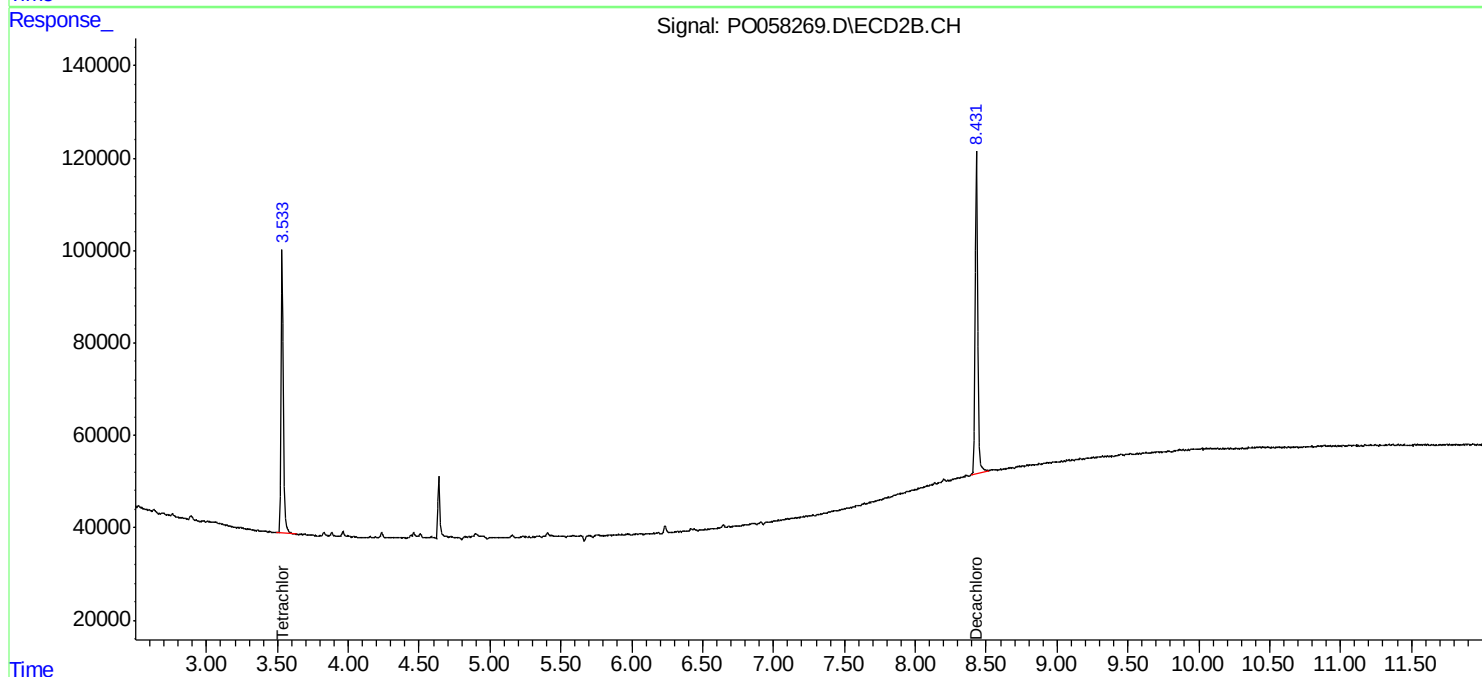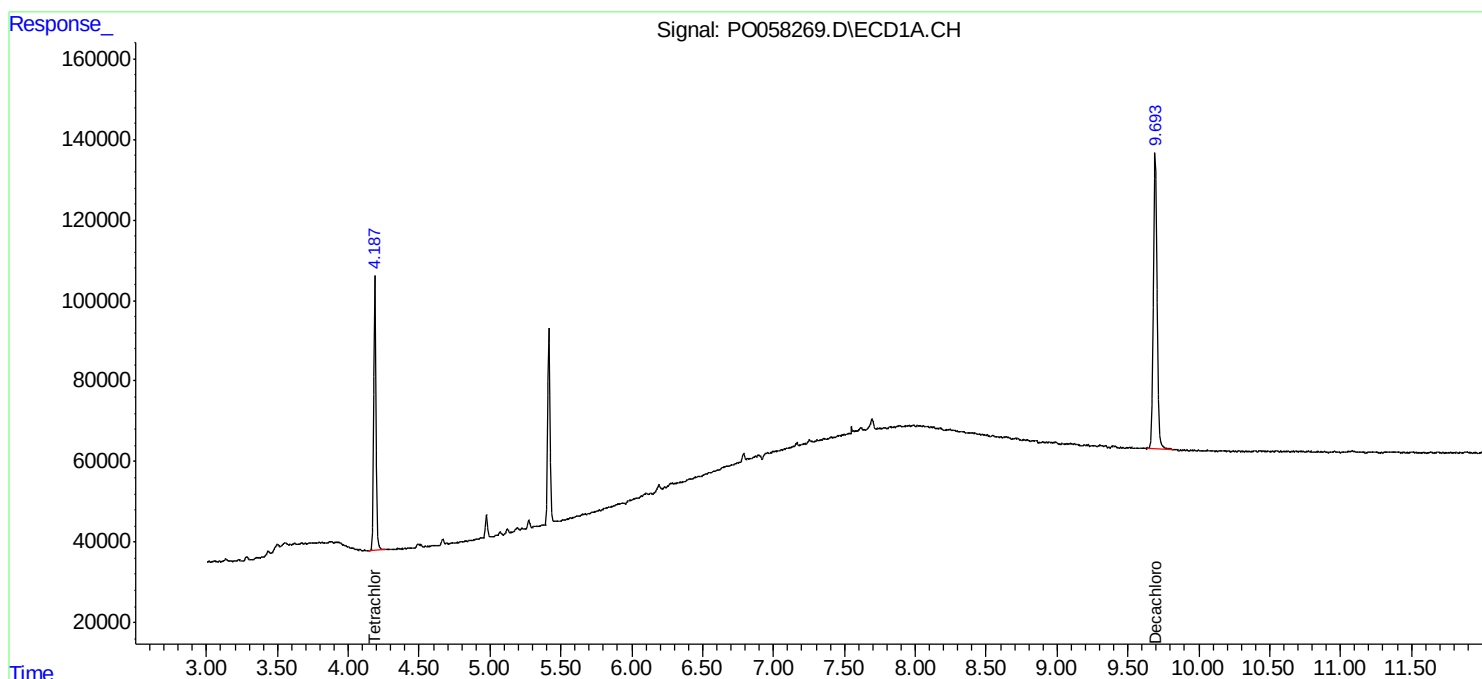


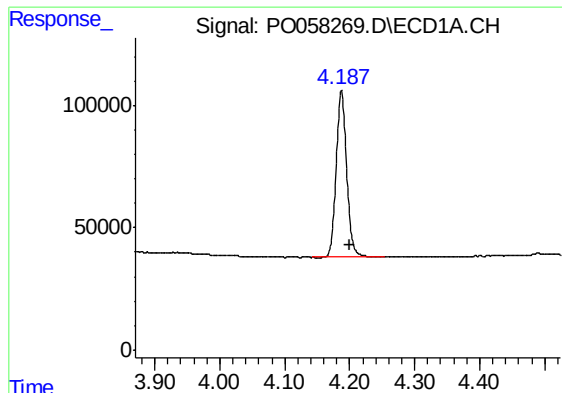

#1 Tetrachloro-m-xylene


R.T.: 4.187 min
Delta R.T.: -0.013 min
Response: 766671
Conc: 22.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-EW03-CONCRETE

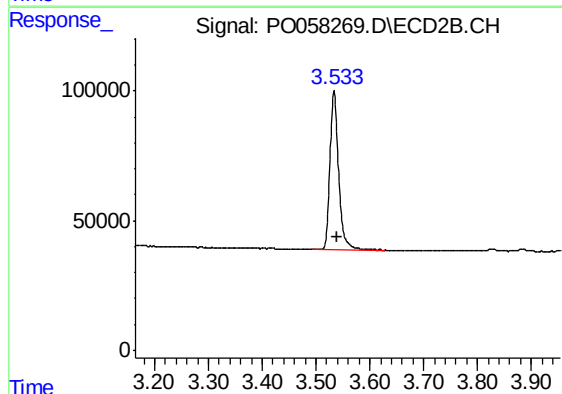


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.006 min
Response: 679414
Conc: 21.18 ng/ml

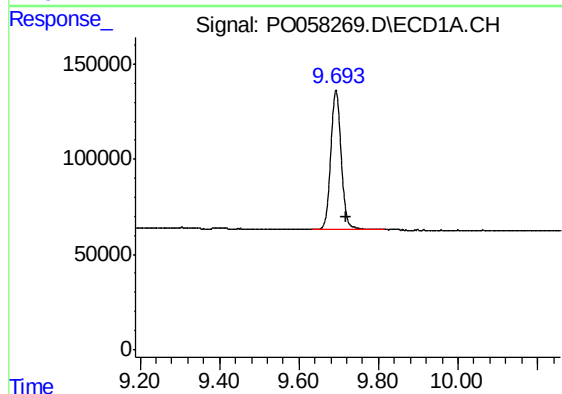

#2 Decachlorobiphenyl

R.T.: 9.693 min
Delta R.T.: -0.025 min
Response: 1340396
Conc: 26.20 ng/ml

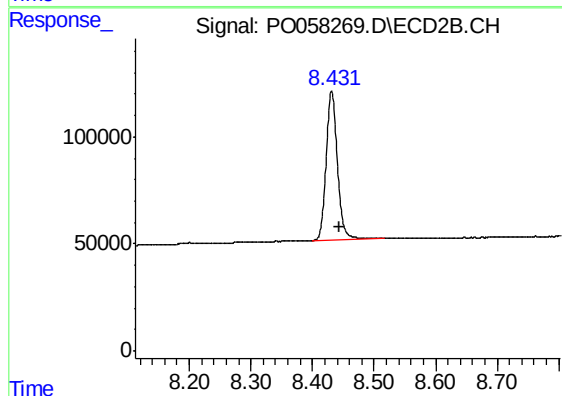

#2 Decachlorobiphenyl

R.T.: 8.432 min
Delta R.T.: -0.014 min
Response: 886183
Conc: 25.85 ng/ml