

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
 Data File : P0058277.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2019 19:23
 Operator : SM/AJ
 Sample : K3834-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TW-3-DEP

Manual Integrations
 APPROVED

Ankita
 7/23/2019 2:24:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 06:00:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.187	3.532	1287944	1094525	38.007	34.125
2)	SA Decachlor...	9.695	8.430	1649723	1118144	32.247m	32.622

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072319\
Data File : P0058277.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2019 19:23
Operator : SM/AJ
Sample : K3834-15
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TW-3-DEP


Manual Integrations
APPROVED

Ankita
7/23/2019 2:24:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 06:00:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

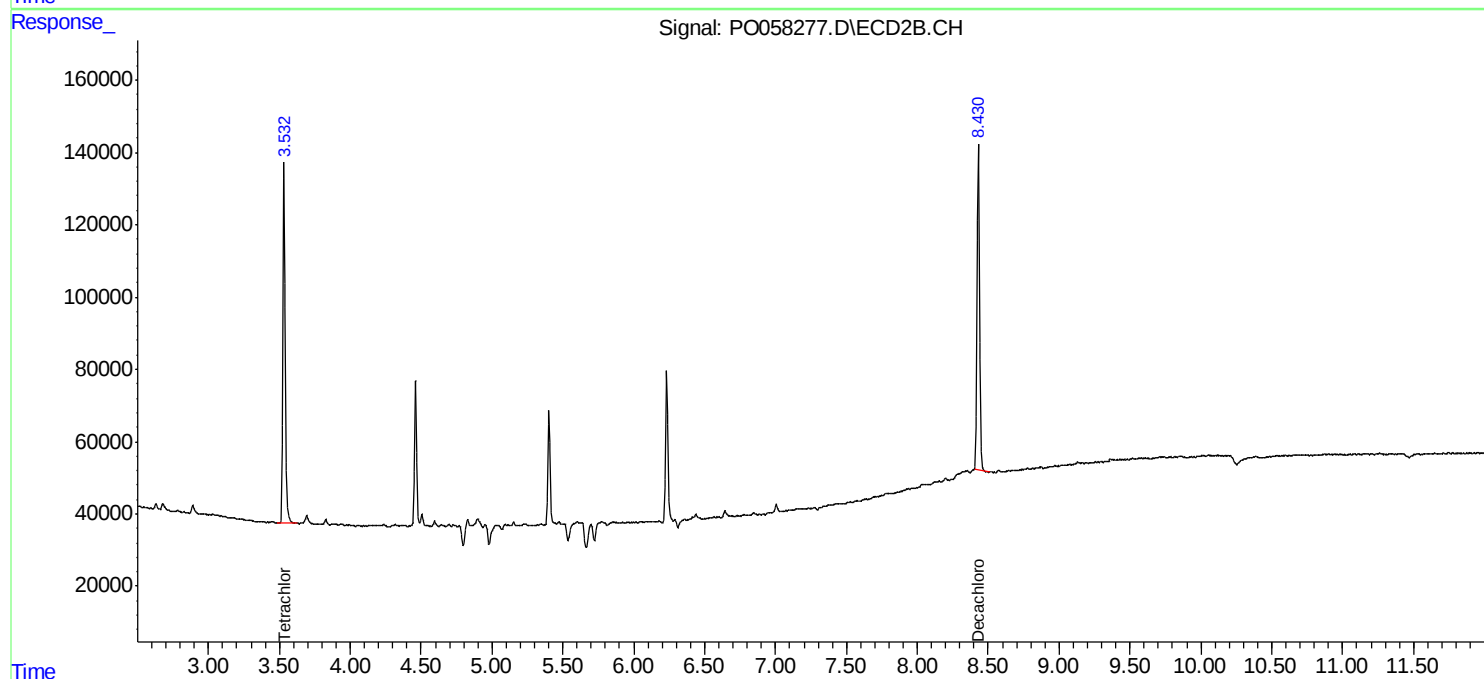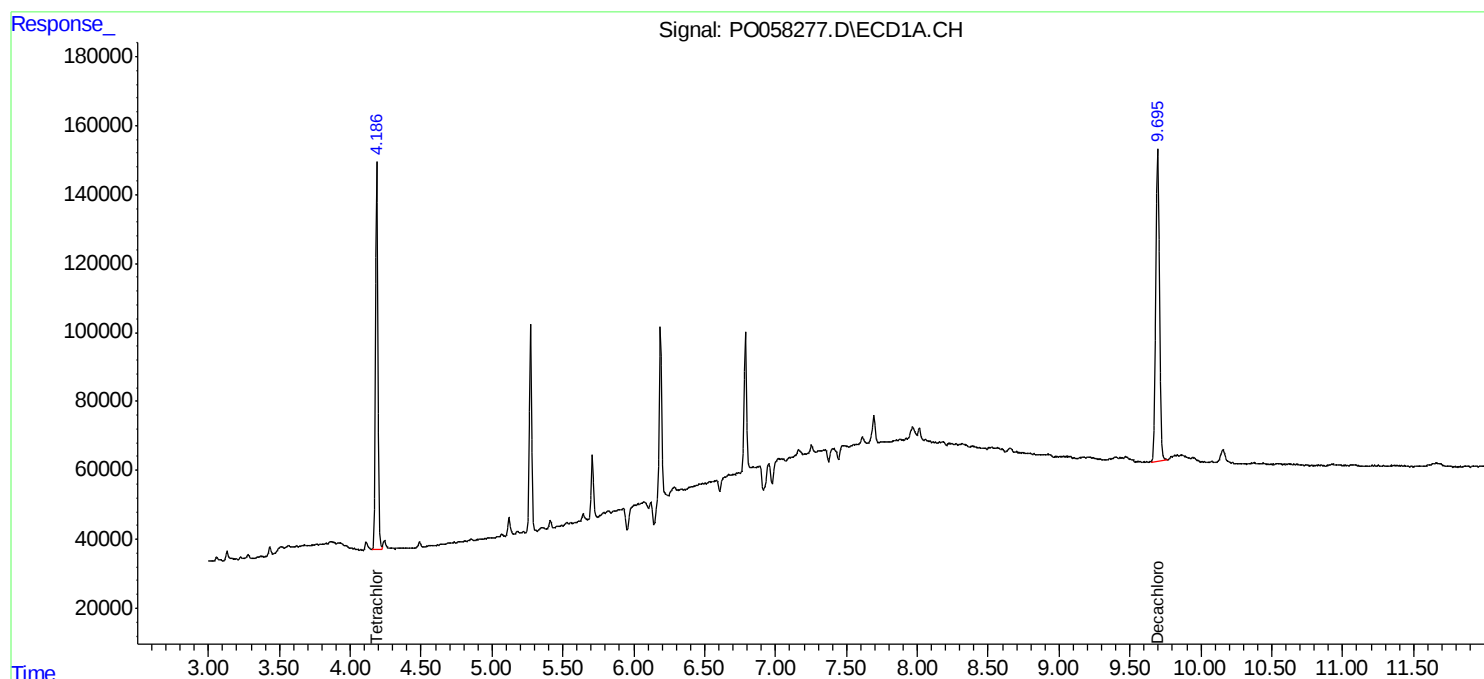

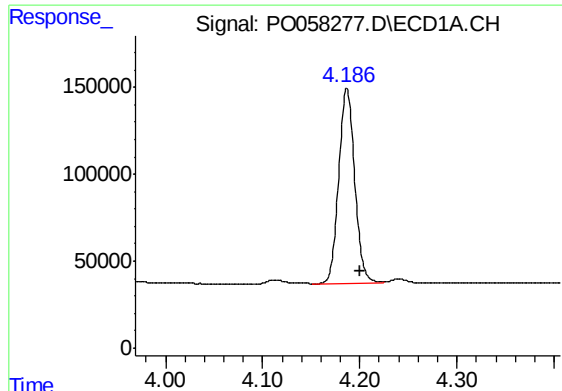


#1 Tetrachloro-m-xylene

R.T.: 4.187 min
Delta R.T.: -0.013 min
Response: 1287944
Conc: 38.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
TW-3-DEP


Manual Integrations
APPROVED

Ankita
7/23/2019 2:24:51 PM

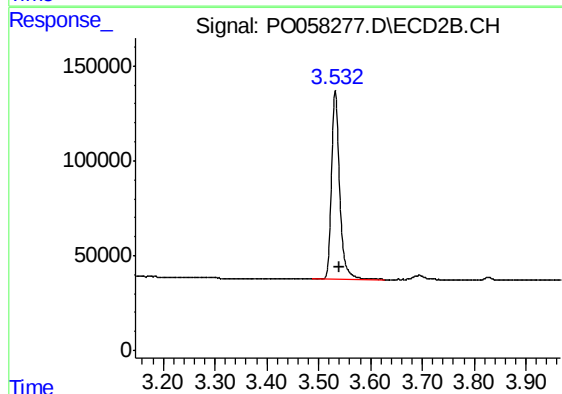


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.007 min
Response: 1094525
Conc: 34.13 ng/ml

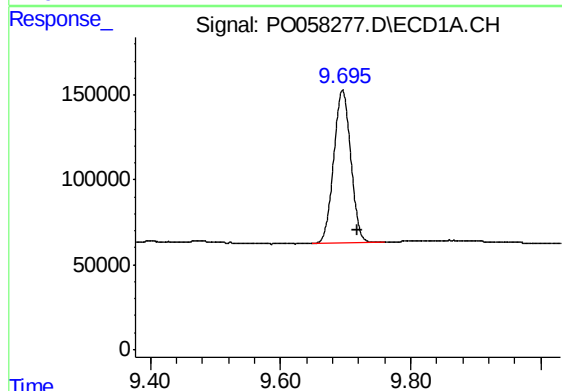

#2 Decachlorobiphenyl

R.T.: 9.695 min
Delta R.T.: -0.023 min
Response: 1649723
Conc: 32.25 ng/ml m

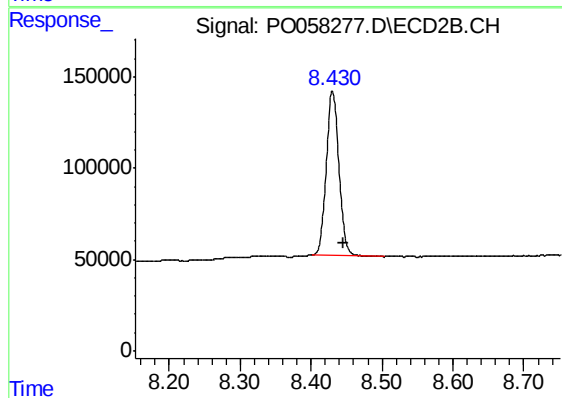

#2 Decachlorobiphenyl

R.T.: 8.430 min
Delta R.T.: -0.015 min
Response: 1118144
Conc: 32.62 ng/ml