

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072419\
 Data File : P0058322.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2019 15:43
 Operator : SM/AJ
 Sample : K3939-11DL 4X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-02-BDL

Manual Integrations
 APPROVED

Ankita
 7/25/2019 3:24:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 15:57:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.191	3.530	215914	196322	6.372	6.121m
2) SA Decachlor...	9.723	8.427	200765	133480	3.924	3.894
Target Compounds						
26) L6 AR-1254-1	6.189	5.376	337256	371953	171.615	182.558
27) L6 AR-1254-2	6.404	5.522	755049	490565	230.969	270.714
28) L6 AR-1254-3	6.770	5.920	1138384	988153	322.690	337.434
29) L6 AR-1254-4	7.054	6.146	1317046	769642	445.125	416.554
30) L6 AR-1254-5	7.471	6.557	1994666	1796899	679.557	660.992

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072419\
Data File : PO058322.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2019 15:43
Operator : SM/AJ
Sample : K3939-11DL 4X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
S2-02-BDL


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 15:57:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

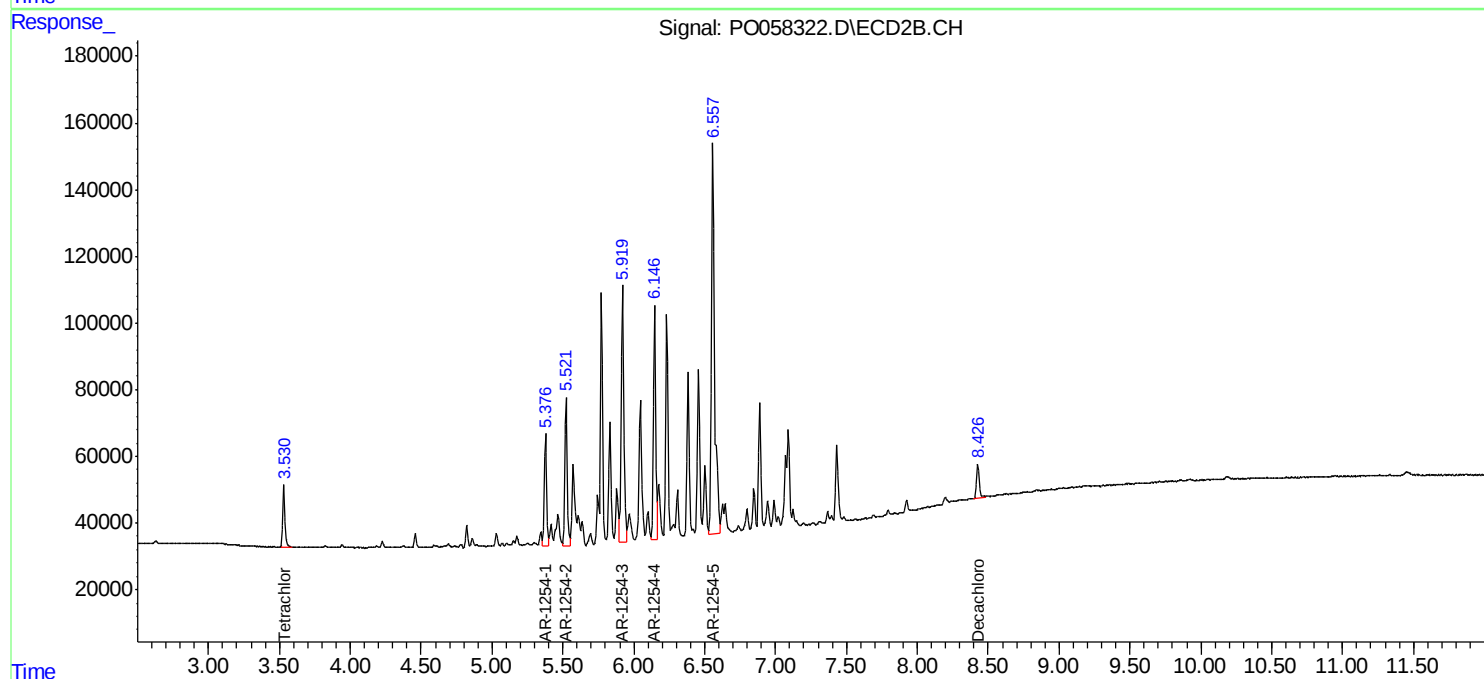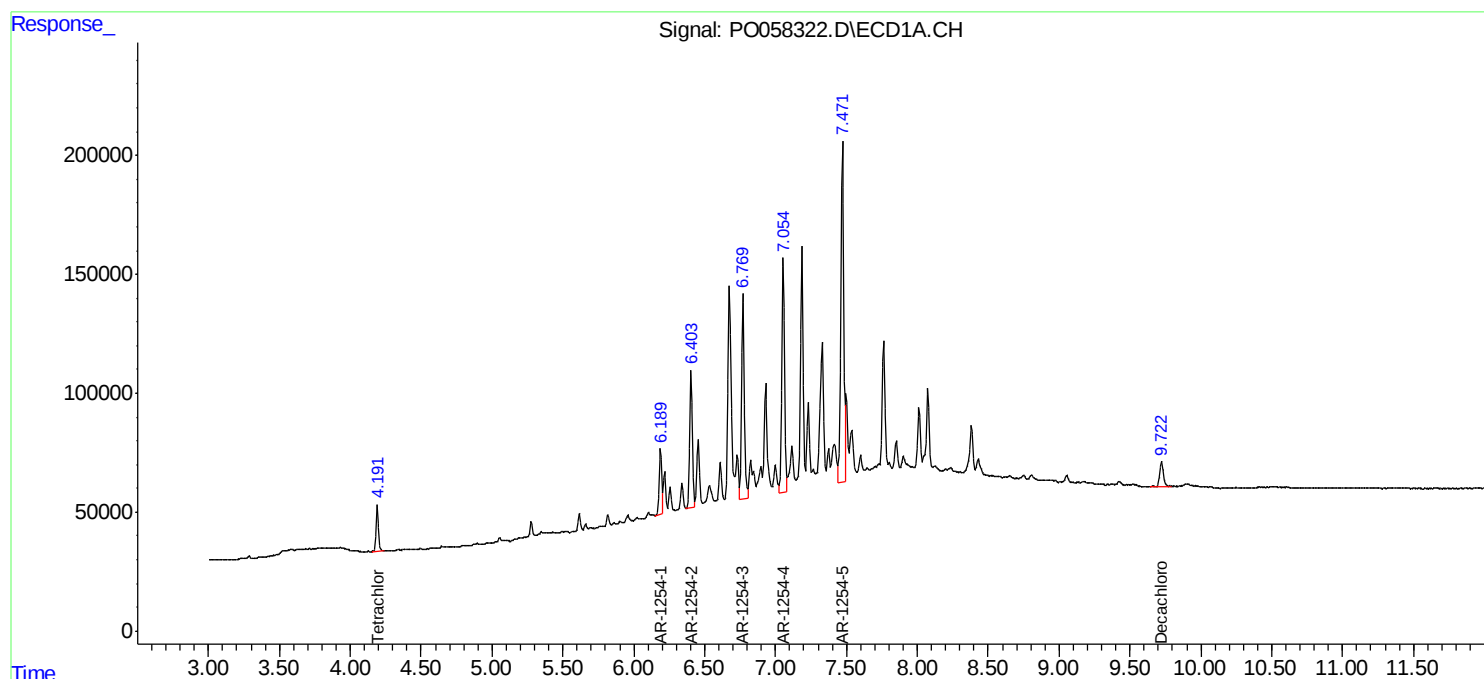

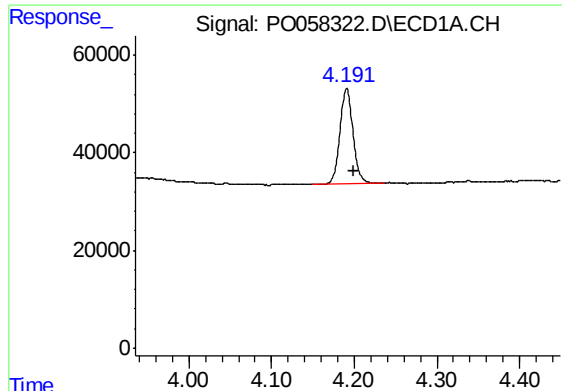


#1 Tetrachloro-m-xylene

R.T.: 4.191 min
Delta R.T.: -0.009 min
Response: 215914
Conc: 6.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-BDL


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:43 PM

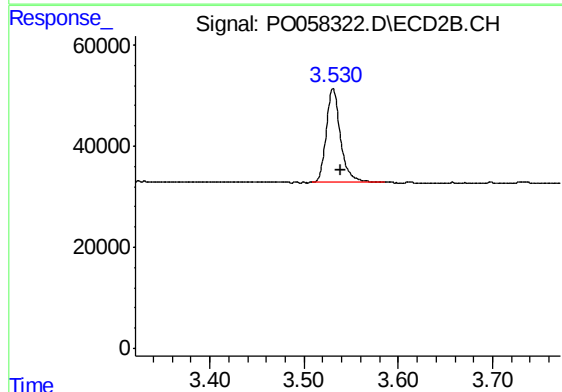


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.009 min
Response: 196322
Conc: 6.12 ng/ml m

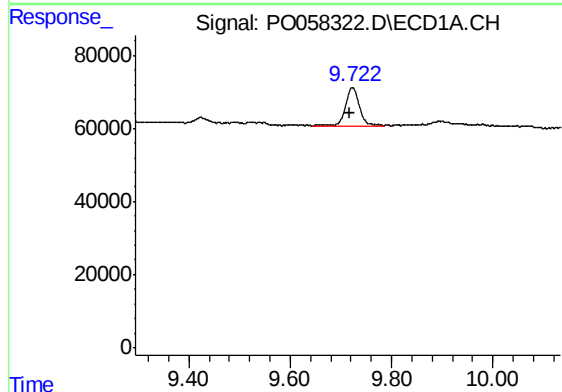


#2 Decachlorobiphenyl

R.T.: 9.723 min
Delta R.T.: 0.005 min
Response: 200765
Conc: 3.92 ng/ml

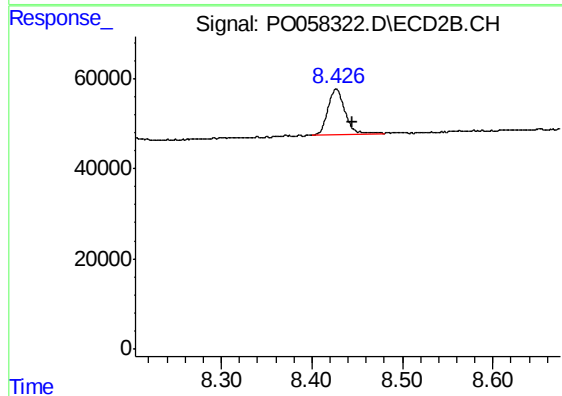

#2 Decachlorobiphenyl

R.T.: 8.427 min
Delta R.T.: -0.018 min
Response: 133480
Conc: 3.89 ng/ml

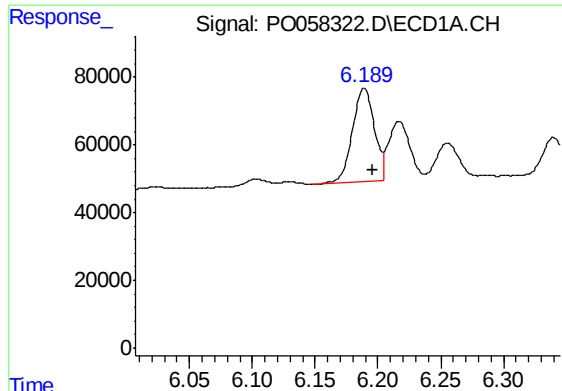


#26 AR-1254-1

R.T.: 6.189 min
Delta R.T.: -0.007 min
Response: 337256
Conc: 171.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-BDL


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:43 PM

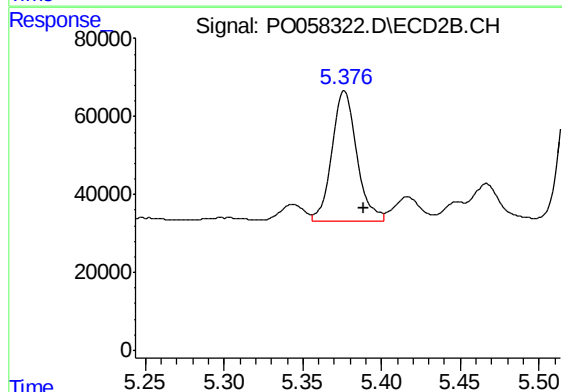


#26 AR-1254-1

R.T.: 5.376 min
Delta R.T.: -0.012 min
Response: 371953
Conc: 182.56 ng/ml

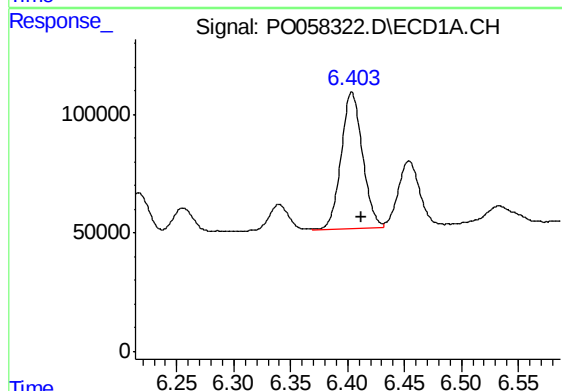


#27 AR-1254-2

R.T.: 6.404 min
Delta R.T.: -0.009 min
Response: 755049
Conc: 230.97 ng/ml

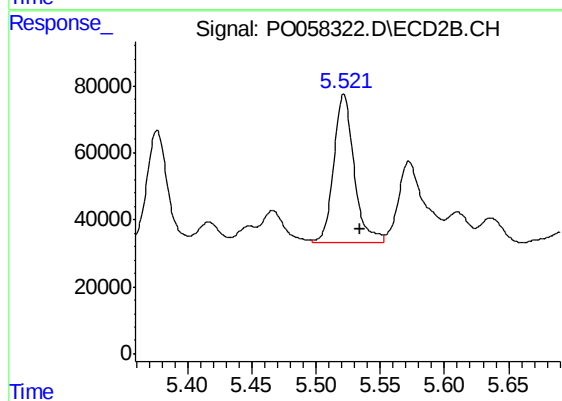

#27 AR-1254-2

R.T.: 5.522 min
Delta R.T.: -0.013 min
Response: 490565
Conc: 270.71 ng/ml

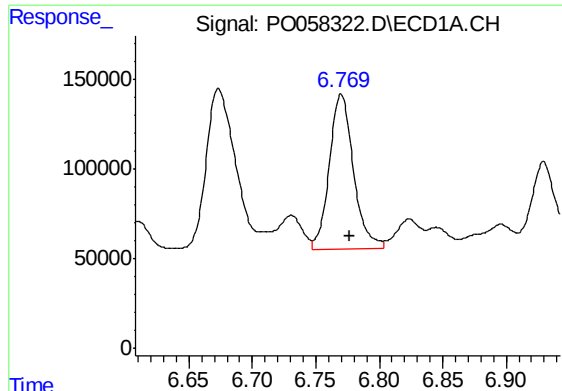


#28 AR-1254-3

R.T.: 6.770 min
Delta R.T.: -0.007 min
Response: 1138384
Conc: 322.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-BDL


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:43 PM

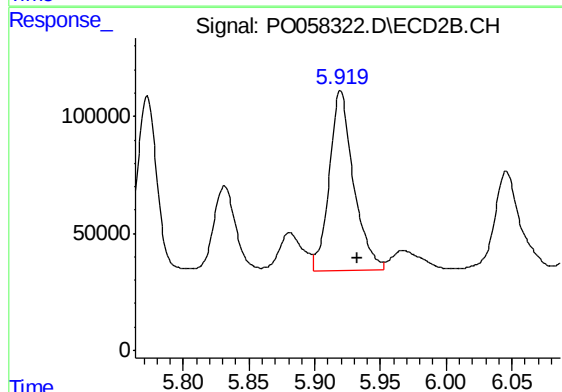


#28 AR-1254-3

R.T.: 5.920 min
Delta R.T.: -0.013 min
Response: 988153
Conc: 337.43 ng/ml

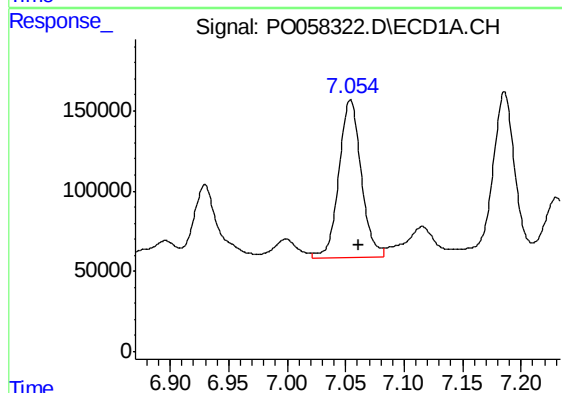


#29 AR-1254-4

R.T.: 7.054 min
Delta R.T.: -0.007 min
Response: 1317046
Conc: 445.12 ng/ml

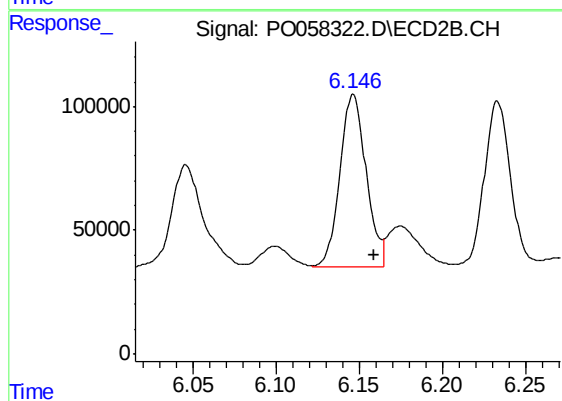

#29 AR-1254-4

R.T.: 6.146 min
Delta R.T.: -0.013 min
Response: 769642
Conc: 416.55 ng/ml

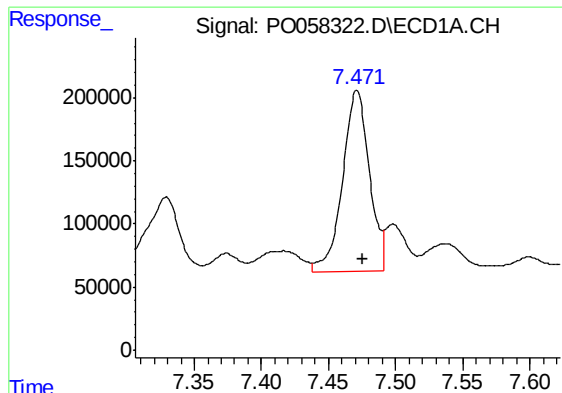


#30 AR-1254-5

R.T.: 7.471 min
Delta R.T.: -0.005 min
Response: 1994666
Conc: 679.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-BDL

Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:43 PM

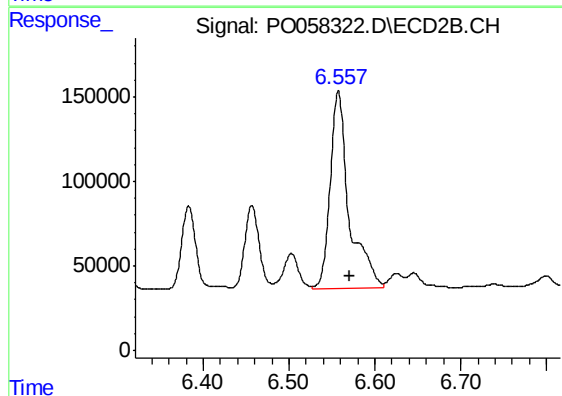

#30 AR-1254-5

R.T.: 6.557 min
Delta R.T.: -0.013 min
Response: 1796899
Conc: 660.99 ng/ml