

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072419\
 Data File : P0058329.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2019 17:52
 Operator : SM/AJ
 Sample : K3617-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-07-071919-A

Manual Integrations
 APPROVED

Ankita
 7/25/2019 3:24:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:06:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.190	3.532	958478	853101	28.285m	26.598
2) SA Decachlor...	9.726	8.429	976726	623952	19.092	18.204

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072419\
Data File : PO058329.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2019 17:52
Operator : SM/AJ
Sample : K3617-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-07-071919-A


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:06:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

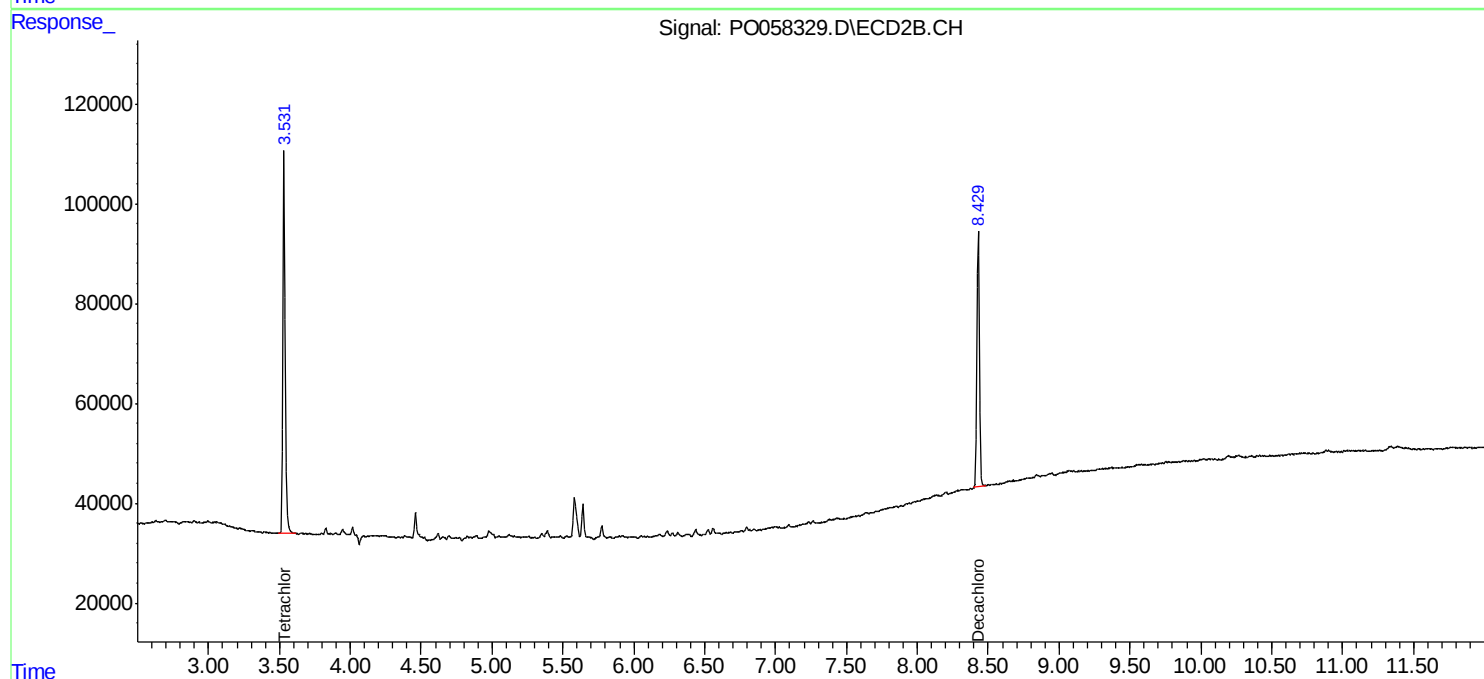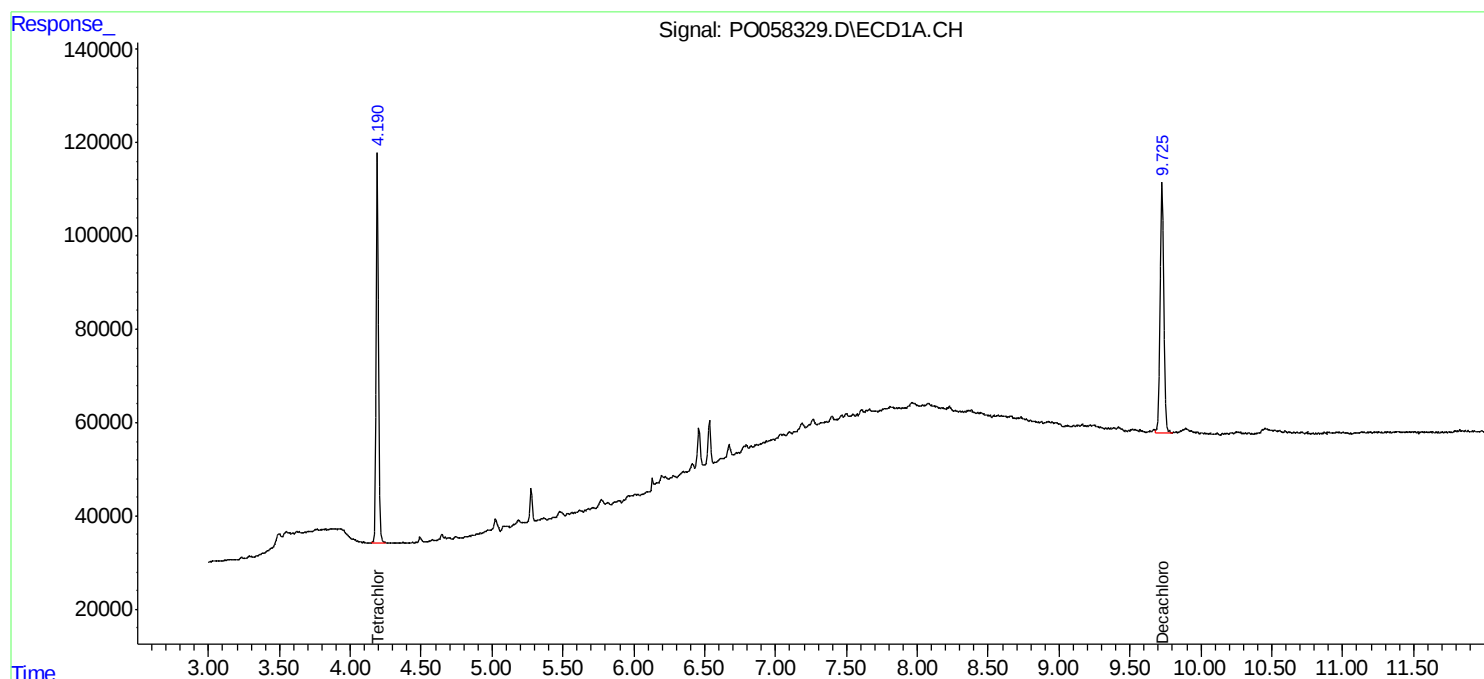

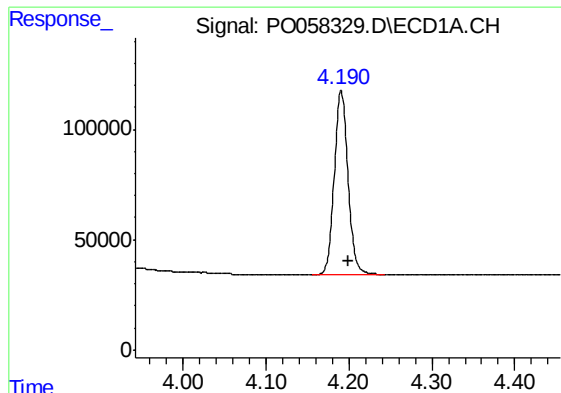


#1 Tetrachloro-m-xylene

R.T.: 4.190 min
Delta R.T.: -0.010 min
Response: 958478
Conc: 28.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
NB-07-071919-A


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:49 PM

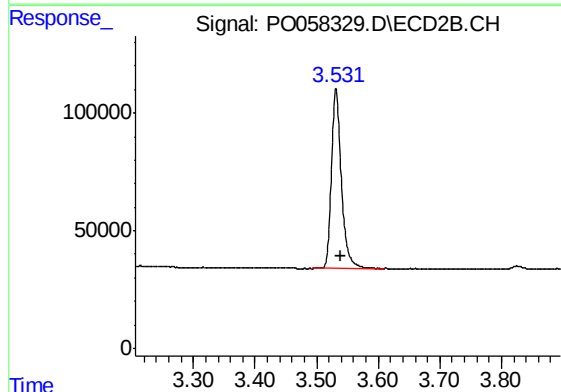


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.008 min
Response: 853101
Conc: 26.60 ng/ml

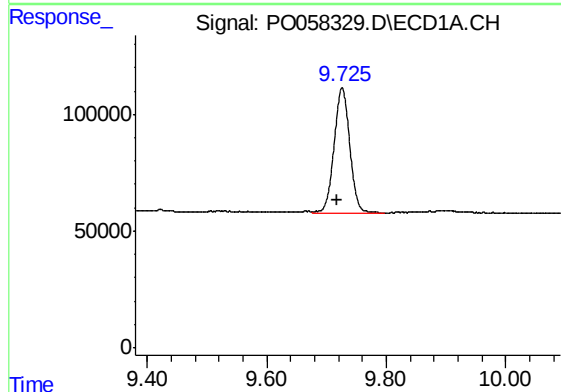

#2 Decachlorobiphenyl

R.T.: 9.726 min
Delta R.T.: 0.008 min
Response: 976726
Conc: 19.09 ng/ml

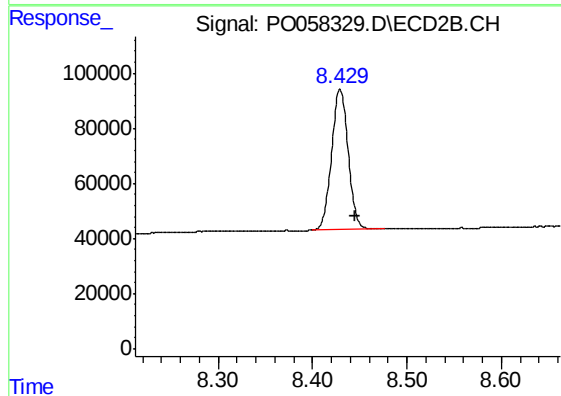

#2 Decachlorobiphenyl

R.T.: 8.429 min
Delta R.T.: -0.016 min
Response: 623952
Conc: 18.20 ng/ml