

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072419\
 Data File : P0058330.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2019 18:08
 Operator : SM/AJ
 Sample : K3617-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-07-071919-B

Manual Integrations
 APPROVED

Ankita
 7/25/2019 3:24:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:07:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.189	3.531	950803	815245	28.058	25.418
2)	SA Decachlor...	9.723	8.427	929974	614436	18.178m	17.926

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072419\
Data File : P0058330.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2019 18:08
Operator : SM/AJ
Sample : K3617-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-07-071919-B


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:07:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

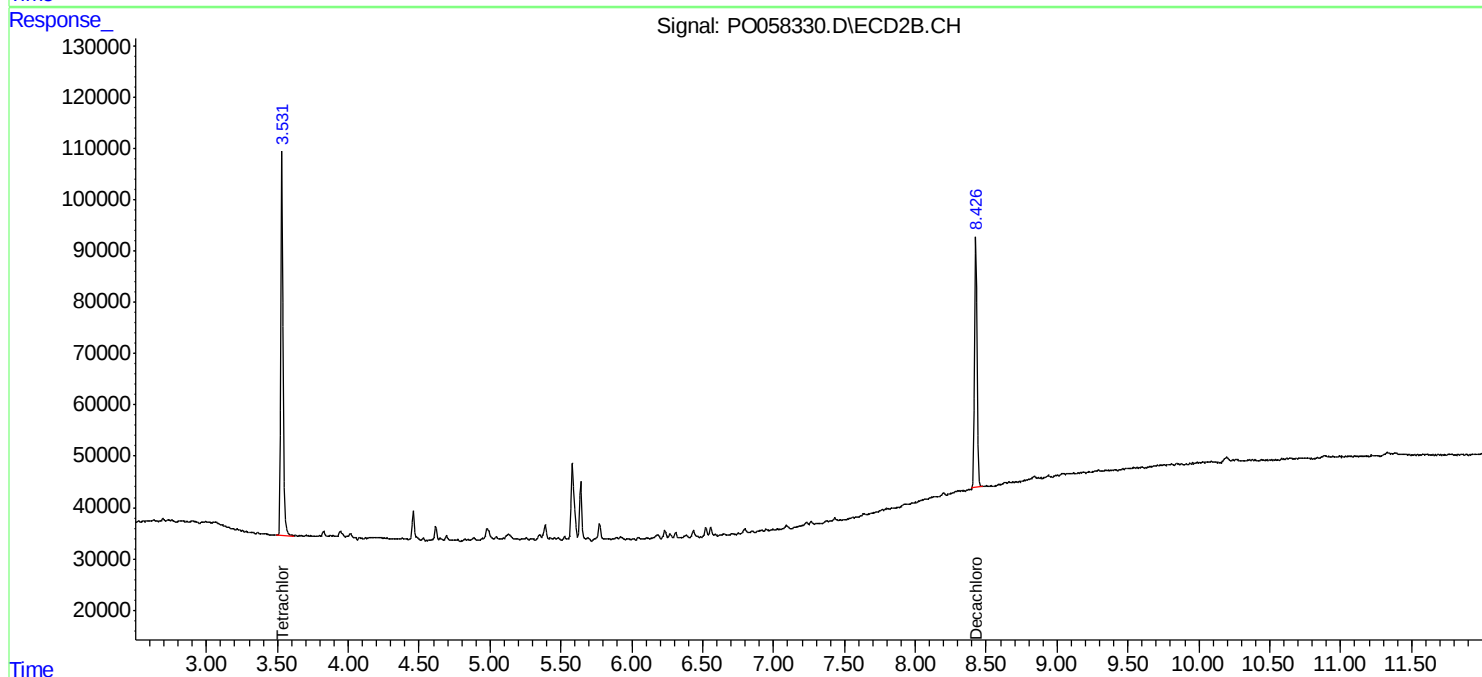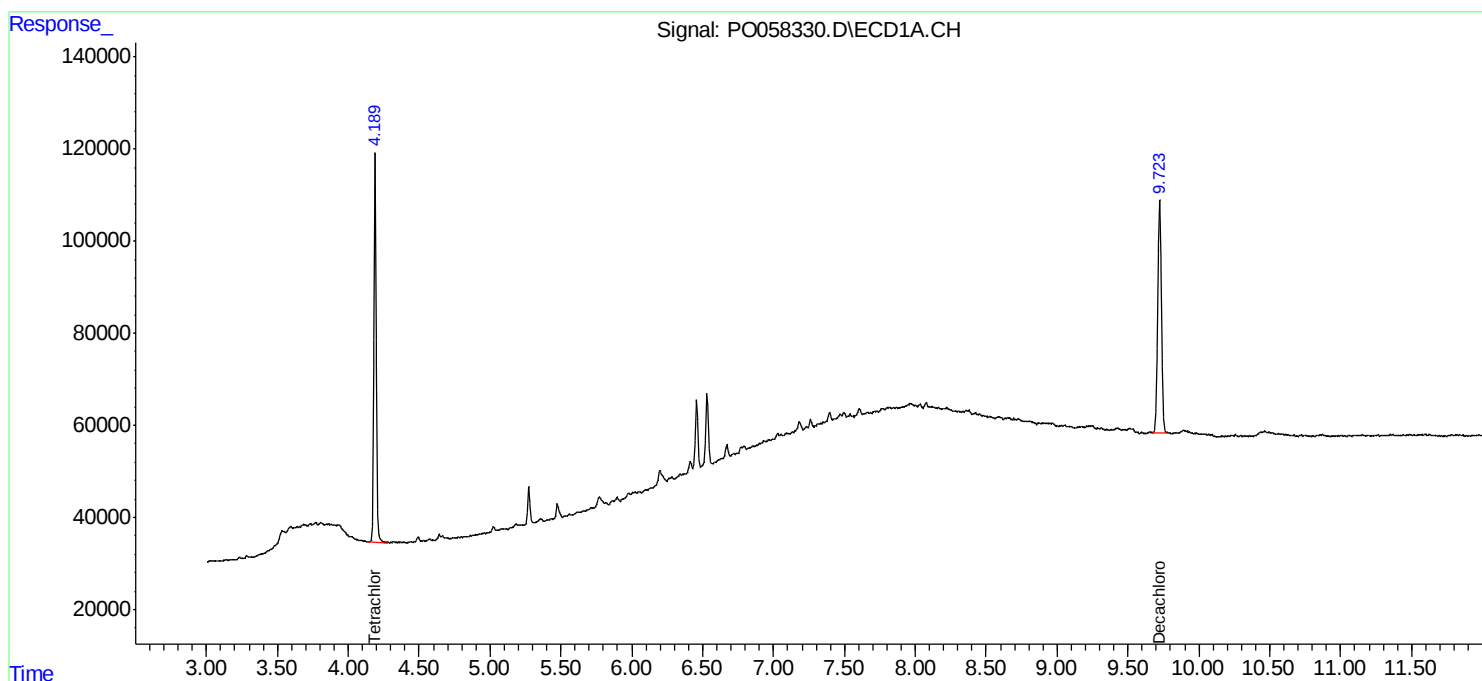

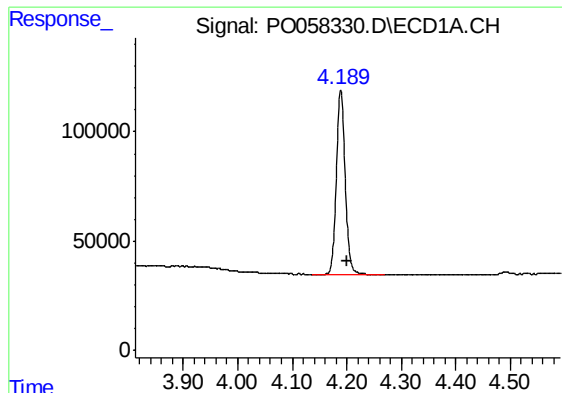


#1 Tetrachloro-m-xylene

R.T.: 4.189 min
Delta R.T.: -0.011 min
Response: 950803
Conc: 28.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-07-071919-B


Manual Integrations
APPROVED

Ankita
7/25/2019 3:24:50 PM

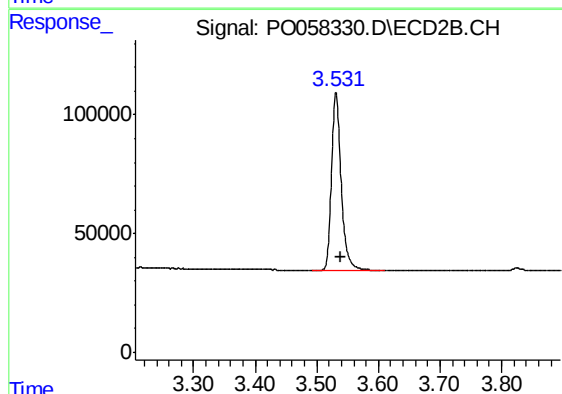


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: -0.008 min
Response: 815245
Conc: 25.42 ng/ml

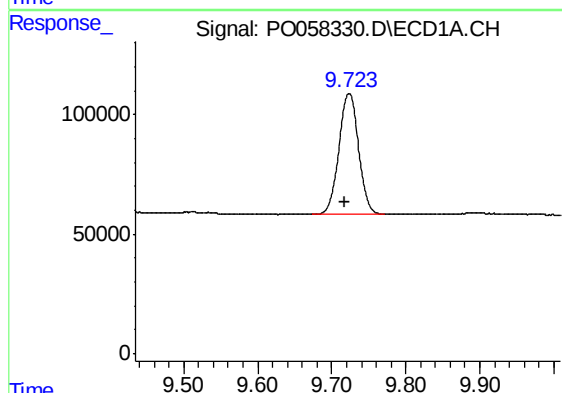

#2 Decachlorobiphenyl

R.T.: 9.723 min
Delta R.T.: 0.005 min
Response: 929974
Conc: 18.18 ng/ml m

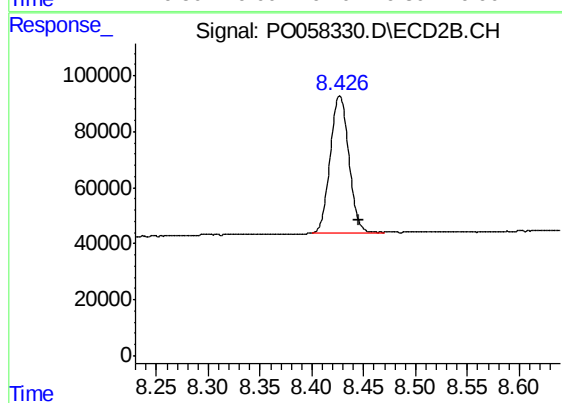

#2 Decachlorobiphenyl

R.T.: 8.427 min
Delta R.T.: -0.018 min
Response: 614436
Conc: 17.93 ng/ml