

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
Data File : P0047119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2018 11:19
Operator : SM/SJ
Sample : J4095-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CON-BALLARDS-0-2

Manual Integrations
APPROVED

Sohil
7/26/2018 4:15:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 11:38:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.647	3027830	3124727	18.059	16.292
2) SA Decachlor...	10.089	8.649	2087099	1828127	19.065	19.905m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
Data File : P0047119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2018 11:19
Operator : SM/SJ
Sample : J4095-03
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CON-BALLARDS-0-2


Manual Integrations
APPROVED

Sohil
7/26/2018 4:15:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 11:38:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

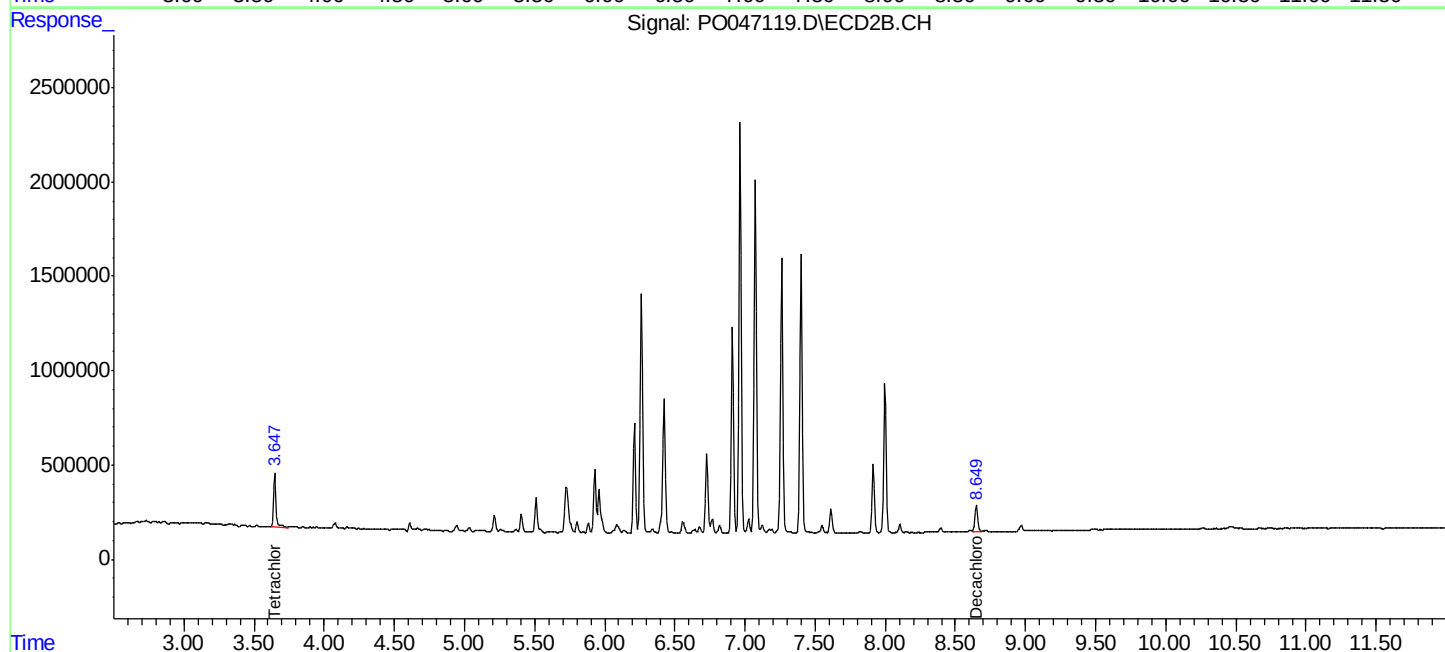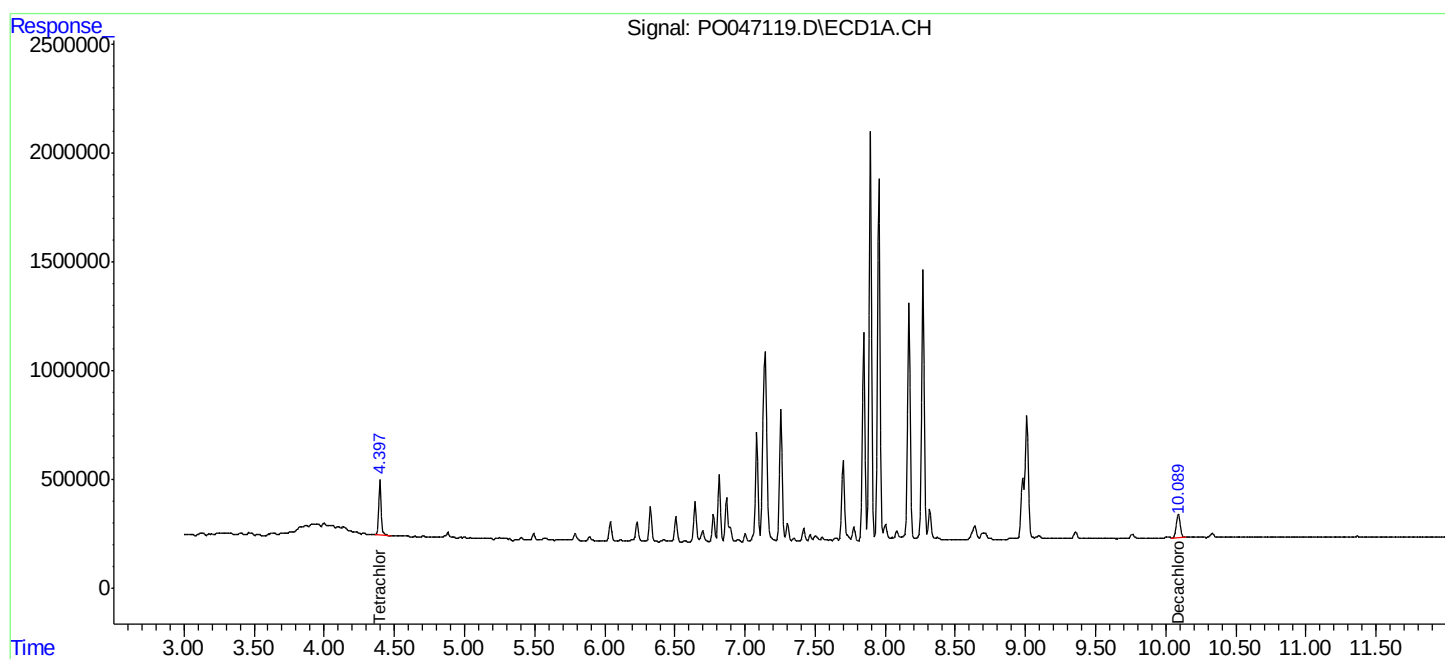

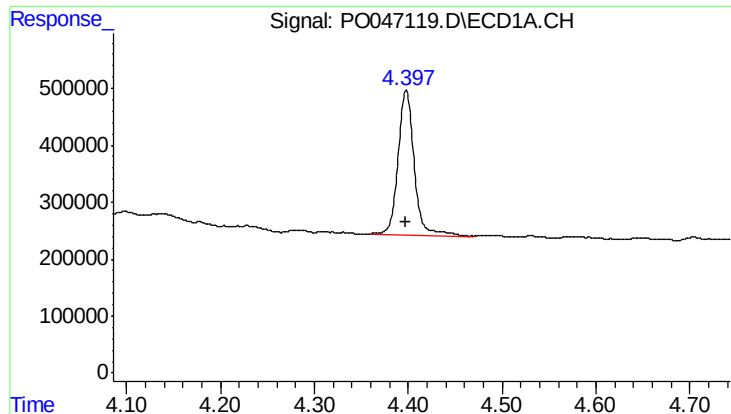


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3027830
Conc: 18.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
CON-BALLARDS-0-2


Manual Integrations
APPROVED

Sohil
7/26/2018 4:15:20 PM

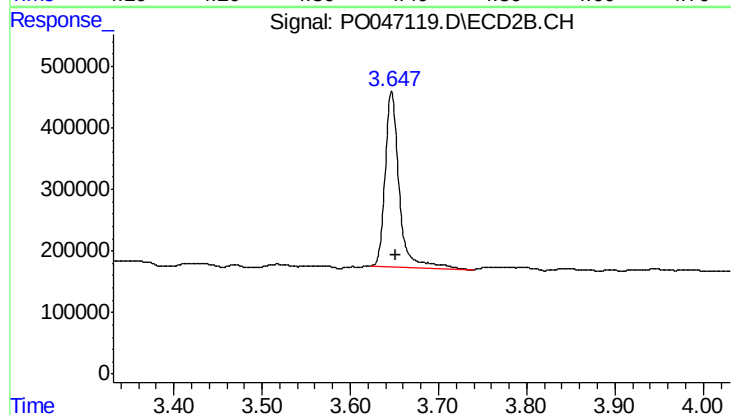


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.004 min
Response: 3124727
Conc: 16.29 ng/ml

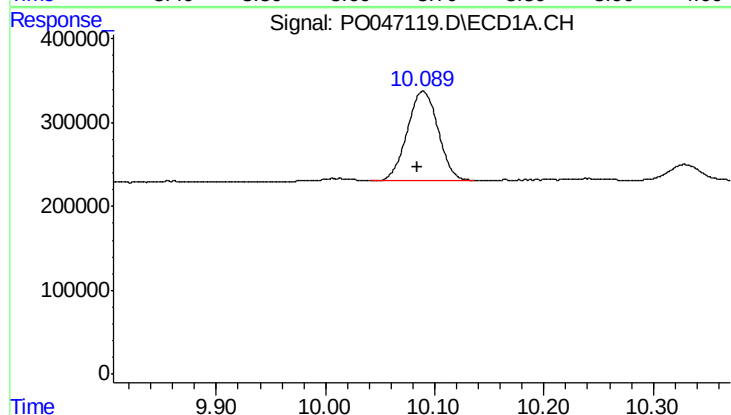

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: 0.005 min
Response: 2087099
Conc: 19.06 ng/ml

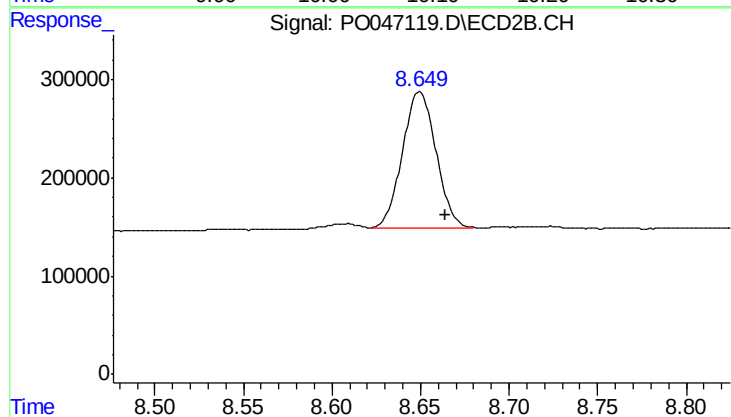

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.015 min
Response: 1828127
Conc: 19.91 ng/ml m