

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
 Data File : P0047120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2018 11:35
 Operator : SM/SJ
 Sample : J4095-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CON-SB-04-05-06-07-0-11

Manual Integrations
 APPROVED

Sohil
 7/26/2018 4:15:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 11:57:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.647	2983926	3287966	17.797	17.143
2) SA Decachlor...	10.090	8.648	1830900	1622380	16.725	17.665m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
Data File : P0047120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2018 11:35
Operator : SM/SJ
Sample : J4095-10
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CON-SB-04-05-06-07-0-11


Manual Integrations
APPROVED

Sohil
7/26/2018 4:15:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 11:57:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

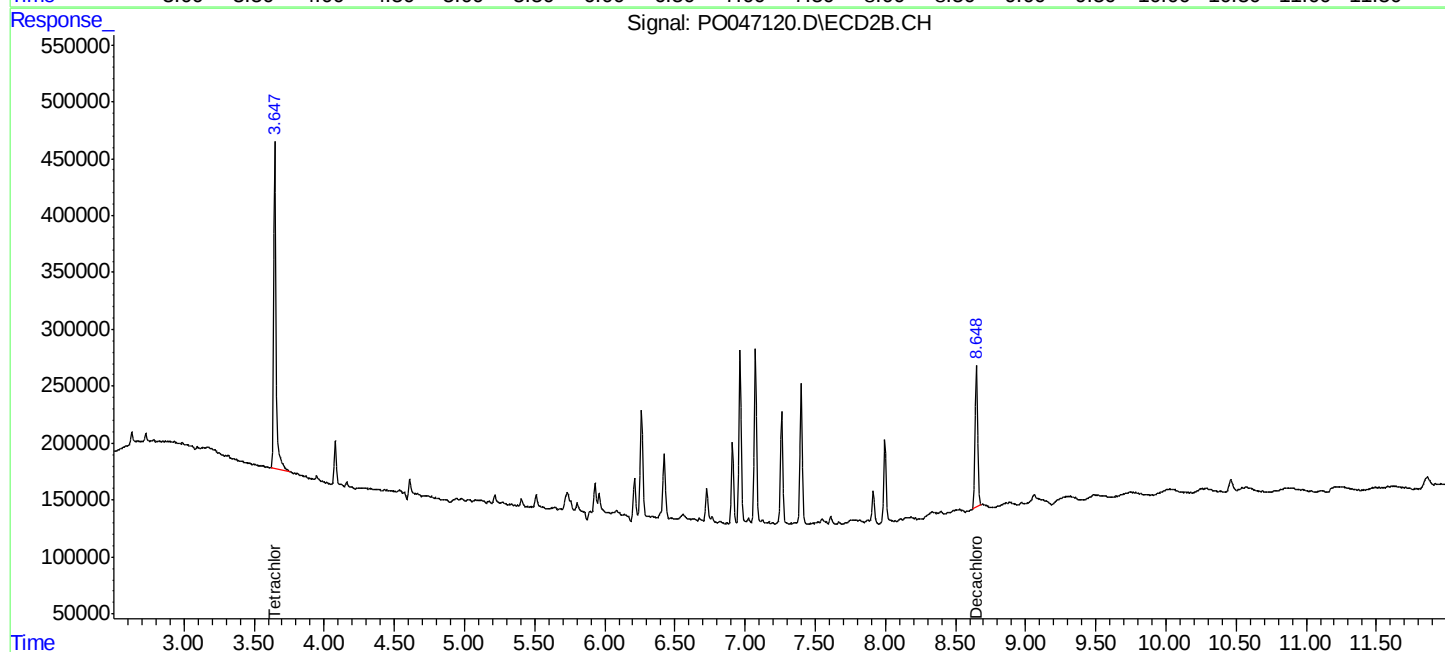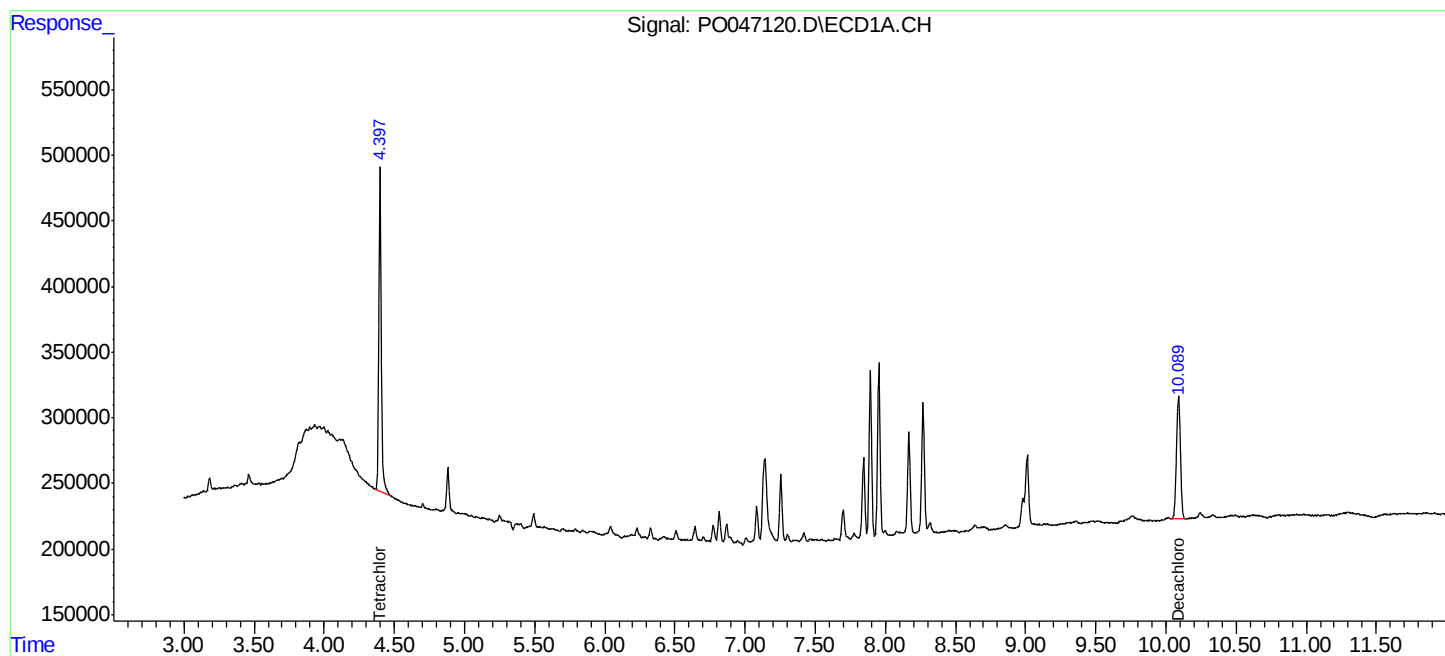

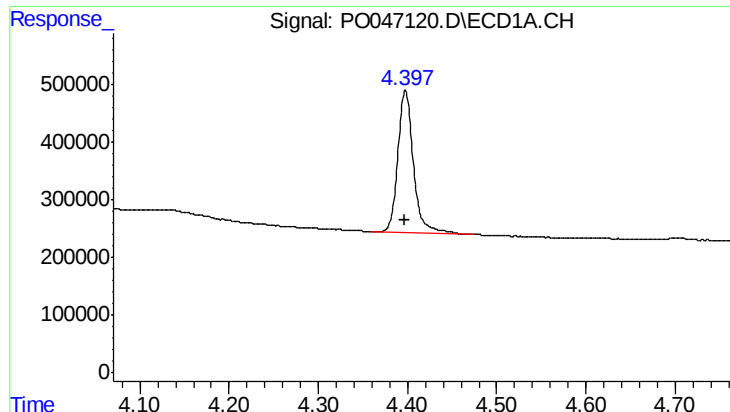


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 2983926
Conc: 17.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
CON-SB-04-05-06-07-0-11


Manual Integrations
APPROVED

Sohil
7/26/2018 4:15:21 PM

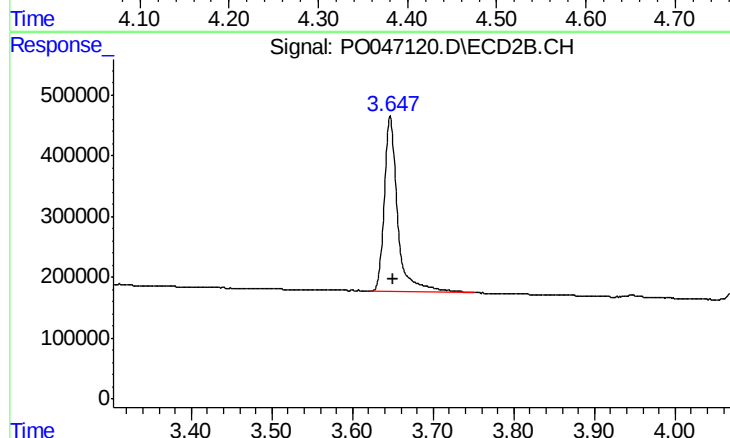


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.004 min
Response: 3287966
Conc: 17.14 ng/ml

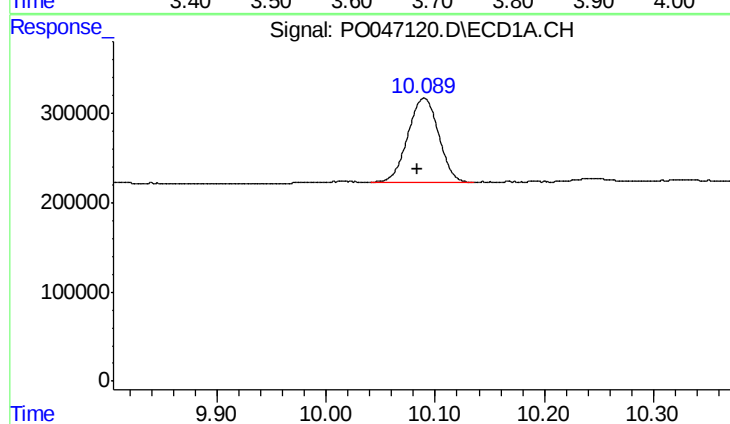

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.006 min
Response: 1830900
Conc: 16.72 ng/ml

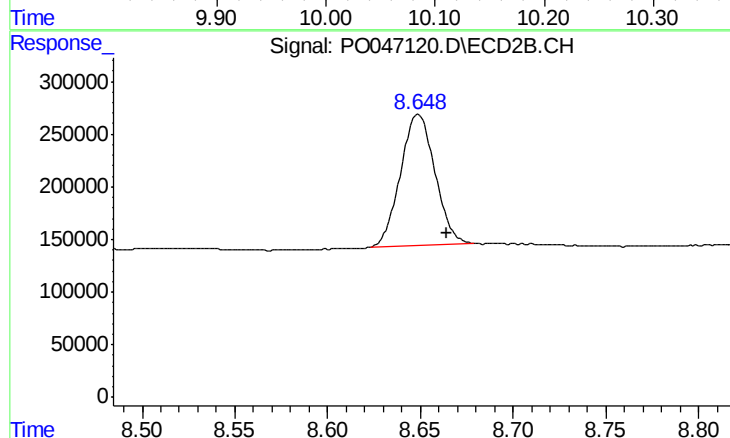

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.016 min
Response: 1622380
Conc: 17.67 ng/ml m