

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
 Data File : P0047163.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2018 23:30
 Operator : SM/SJ
 Sample : J4133-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 072318-TIPC-E-D-M

Manual Integrations
 APPROVED

Sohil
 7/26/2018 4:17:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:27:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.645	3640626	3322355	21.713m	17.322m
2) SA Decachlor...	10.090	8.648	2299101	2100415	21.001	22.870

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
Data File : P0047163.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2018 23:30
Operator : SM/SJ
Sample : J4133-07
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
072318-TIPC-E-D-M


Manual Integrations
APPROVED

Sohil
7/26/2018 4:17:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:27:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

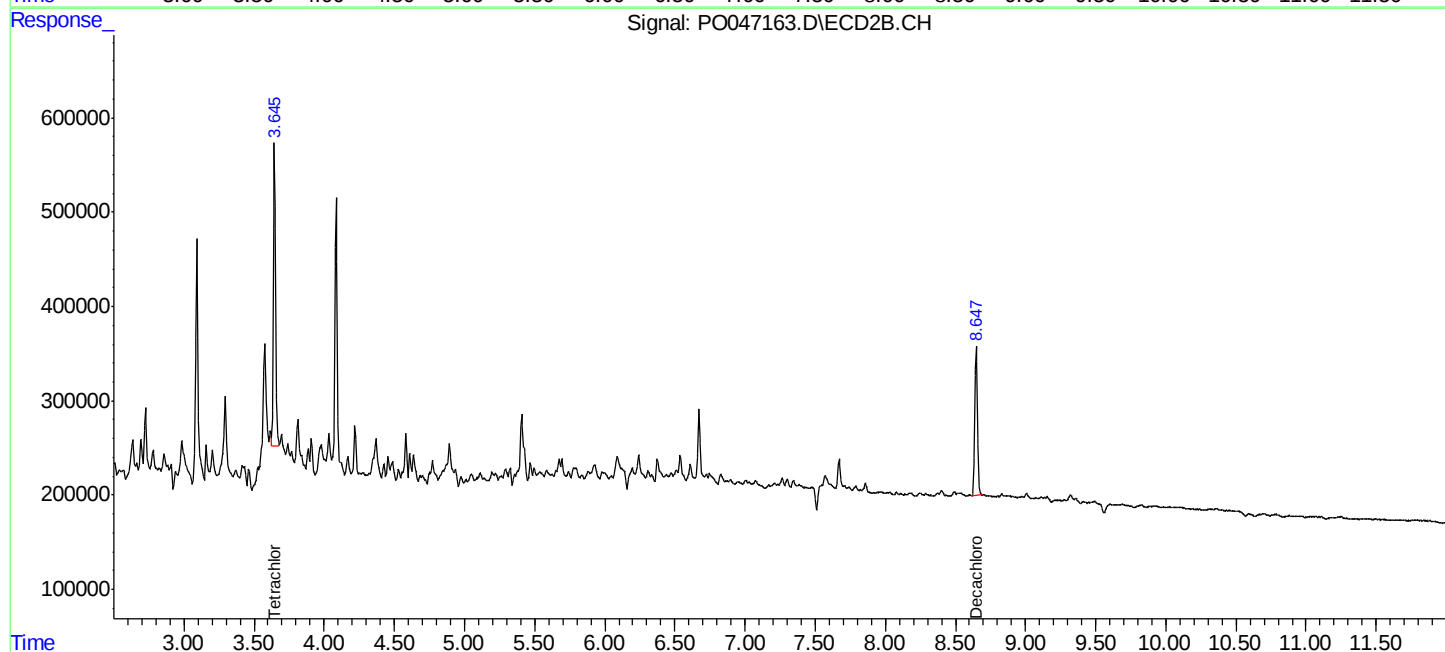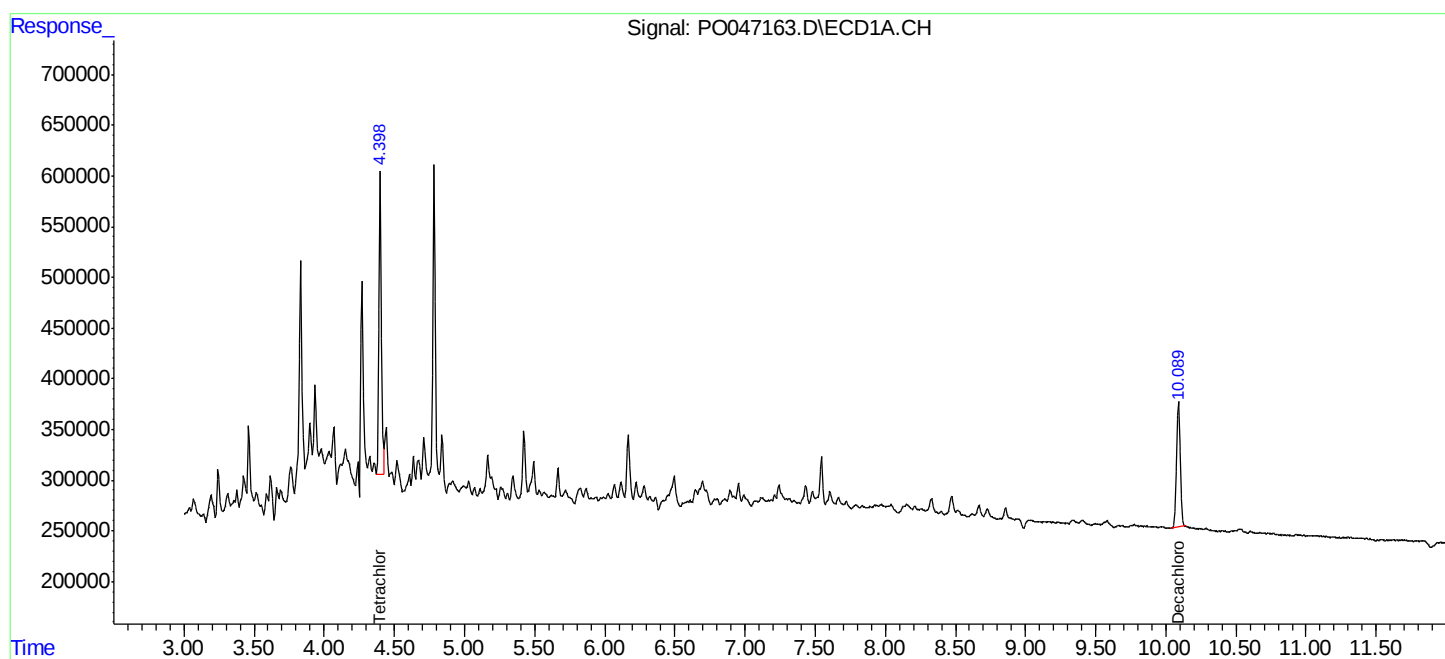

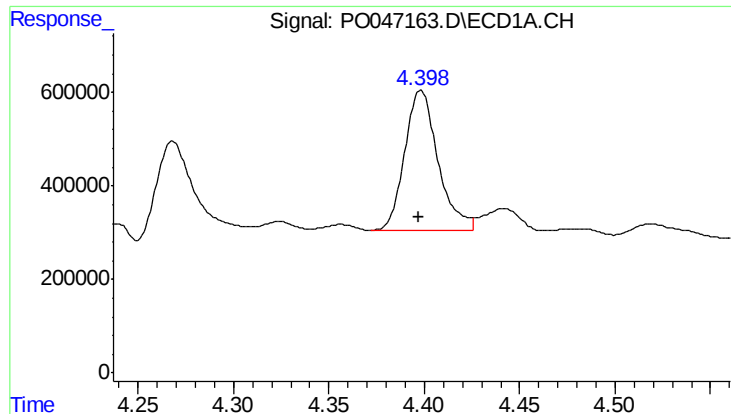


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3640626
Conc: 21.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
072318-TIPC-E-D-M


Manual Integrations
APPROVED

Sohil
7/26/2018 4:17:14 PM

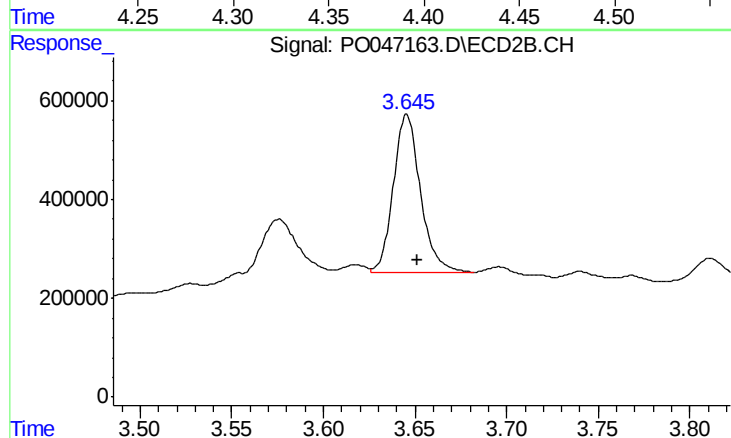


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.006 min
Response: 3322355
Conc: 17.32 ng/ml m

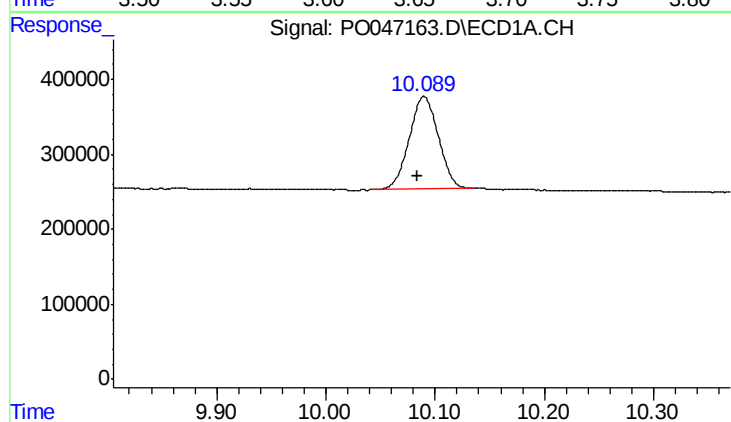

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.006 min
Response: 2299101
Conc: 21.00 ng/ml

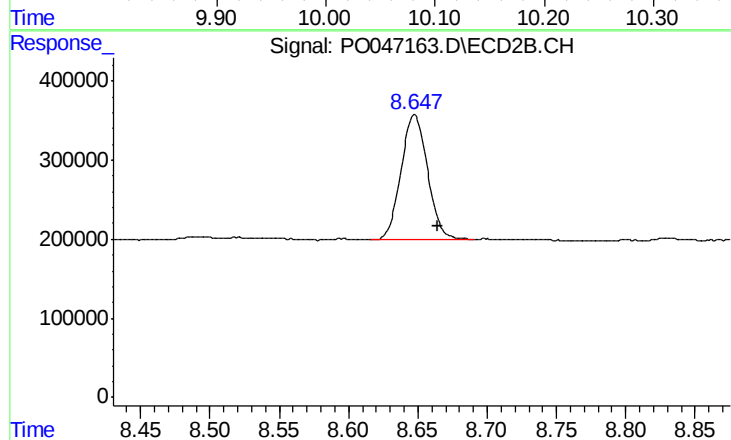

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.017 min
Response: 2100415
Conc: 22.87 ng/ml