

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
 Data File : P0047167.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jul 2018 1:22
 Operator : SM/SJ
 Sample : J4076-01RE
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SD-LT05-01-A-18RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 03:38:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.645	2504621	2892501	14.938	15.081
2) SA Decachlor...	10.091	8.648	930894	887471	8.503	9.663

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072518\
Data File : P0047167.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jul 2018 1:22
Operator : SM/SJ
Sample : J4076-01RE
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SD-LT05-01-A-18RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 03:38:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

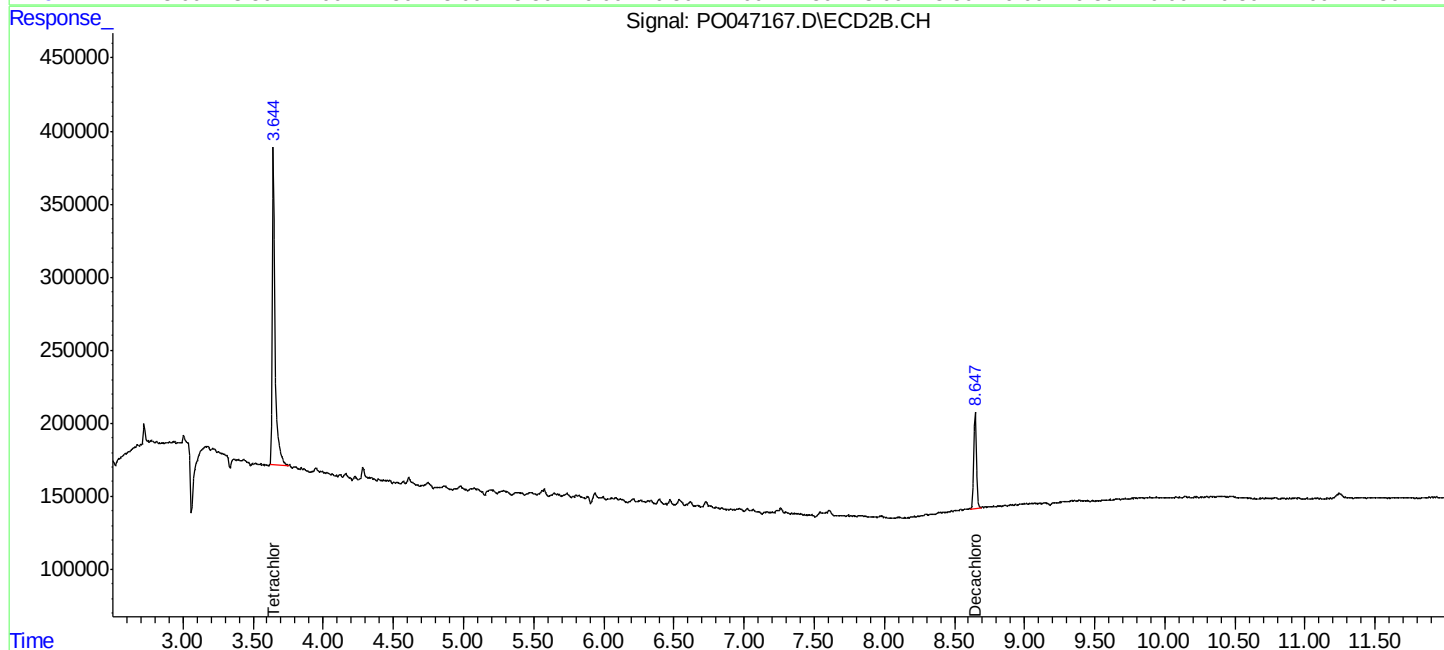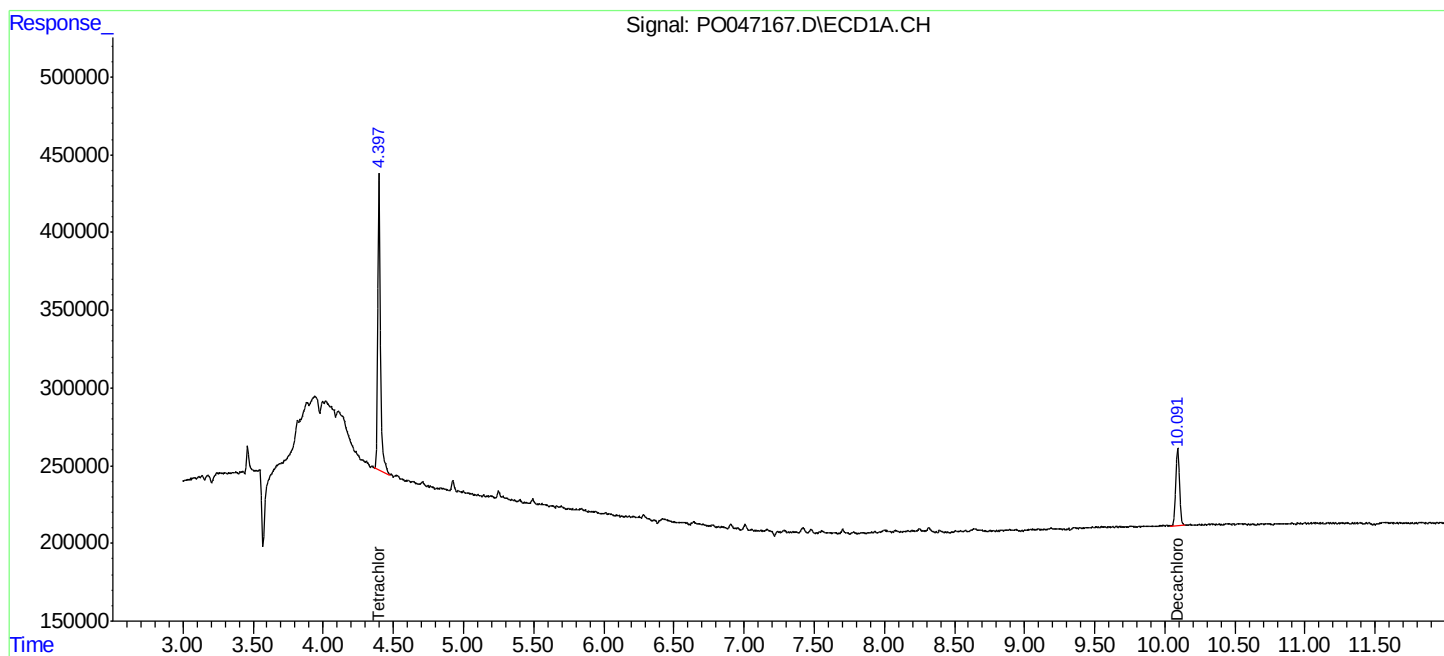


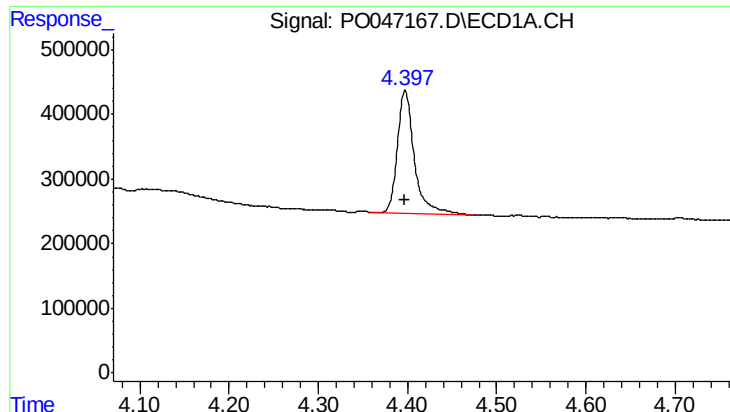

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 2504621
Conc: 14.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
SD-LT05-01-A-18RE

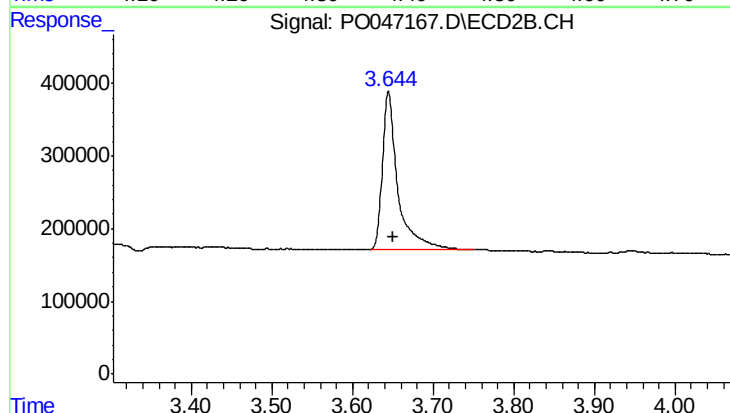


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.006 min
Response: 2892501
Conc: 15.08 ng/ml

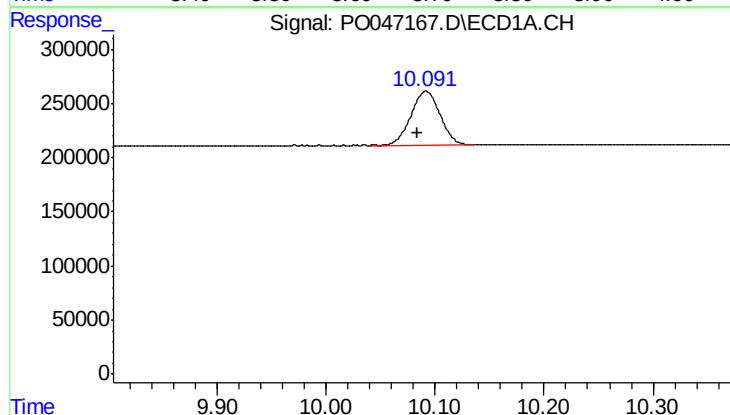

#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: 0.007 min
Response: 930894
Conc: 8.50 ng/ml

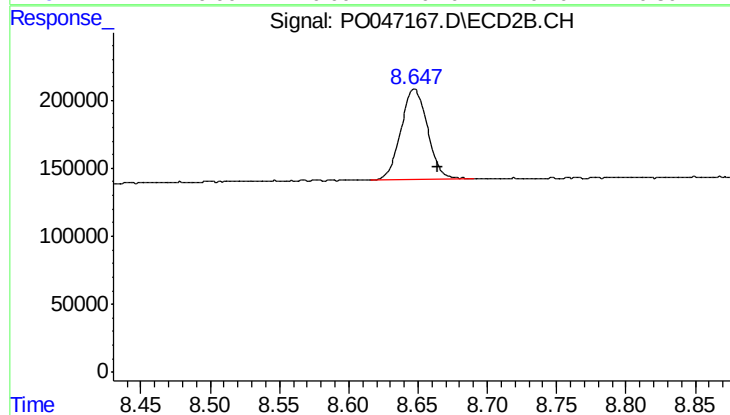

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.017 min
Response: 887471
Conc: 9.66 ng/ml