

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
Data File : P0058363.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2019 18:08
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Ankita
7/25/2019 2:00:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 01:20:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.188	3.529	622973	600245	18.384m	18.715
2) SA Decachlor...	9.691	8.427	864823	564582	16.905m	16.472

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
Data File : P0058363.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2019 18:08
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
7/25/2019 2:00:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 01:20:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

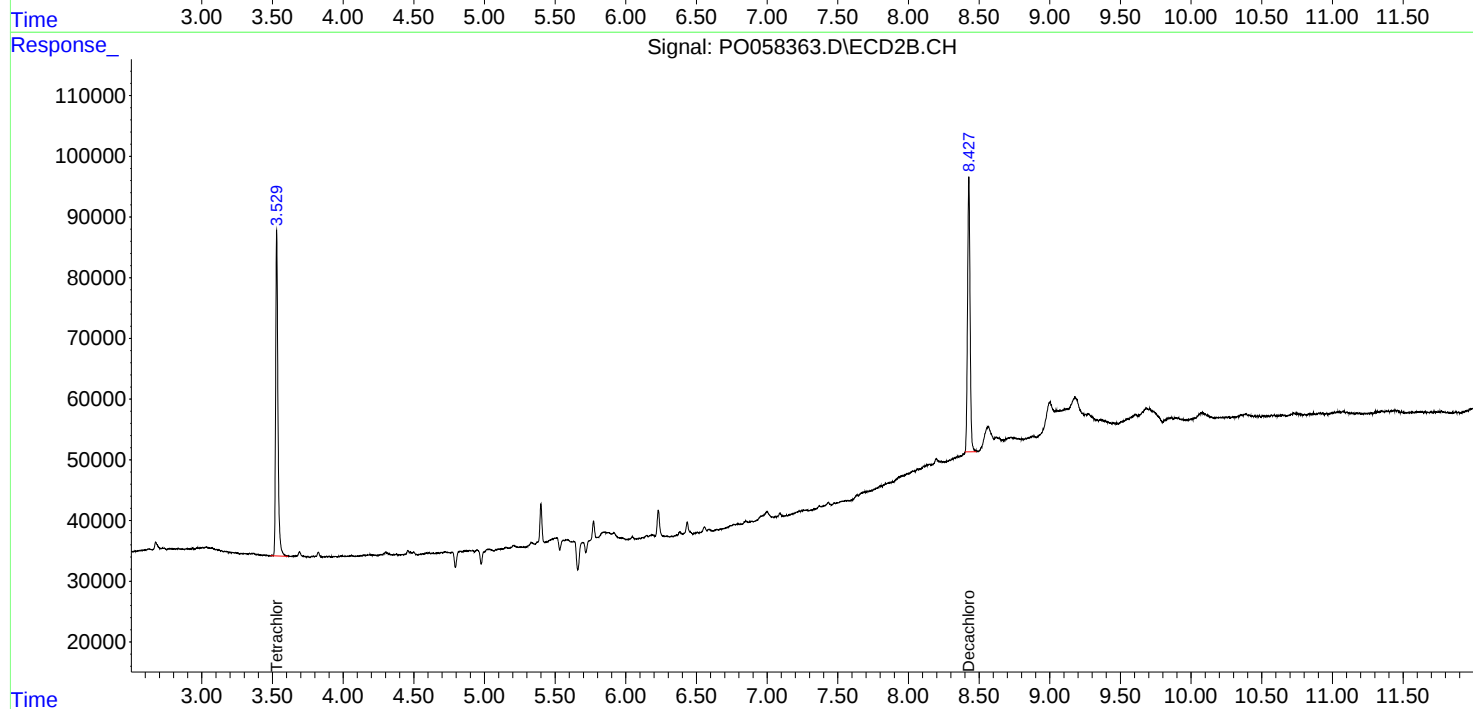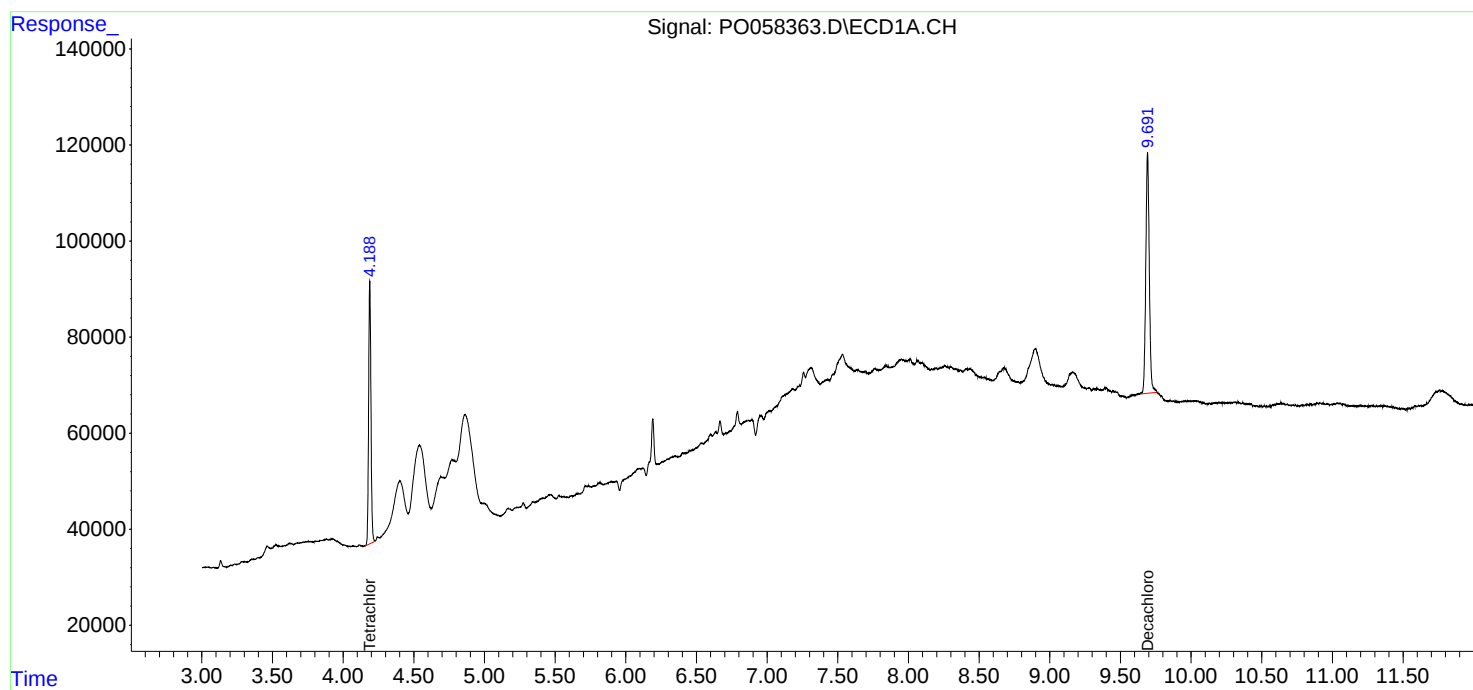

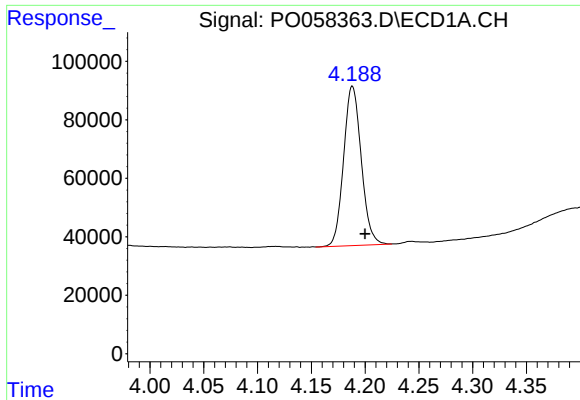


#1 Tetrachloro-m-xylene

R.T.: 4.188 min
Delta R.T.: -0.012 min
Response: 622973
Conc: 18.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
7/25/2019 2:00:07 PM

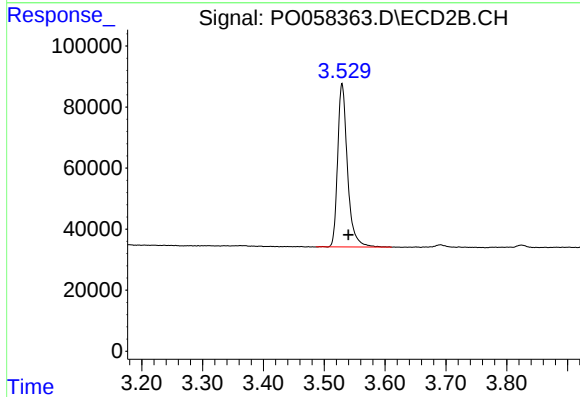


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.010 min
Response: 600245
Conc: 18.71 ng/ml

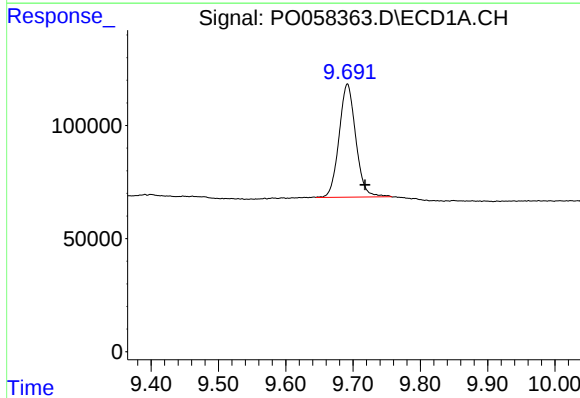

#2 Decachlorobiphenyl

R.T.: 9.691 min
Delta R.T.: -0.027 min
Response: 864823
Conc: 16.90 ng/ml m

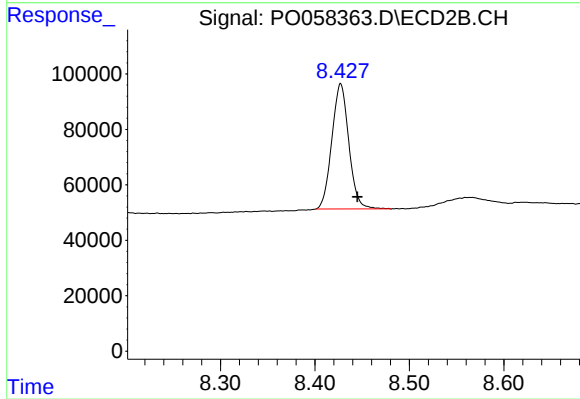

#2 Decachlorobiphenyl

R.T.: 8.427 min
Delta R.T.: -0.018 min
Response: 564582
Conc: 16.47 ng/ml